

Instructions for use



lina
PR013-003-17
PR013-003-22

Symbols

Symbols displayed on the product and/or used in this manual:



WARNING!
Risk of injury



ATTENTION!
To prevent damage occurring



General explanations,
without risk to persons or objects



HOT SURFACES!
Risk of burns



HOT STEAM!
Risk of burns



Call service



Thermo washer
disinfectable



Consult instruction for use



Do not dispose of
with normal waste



Do not use tap water
to fill the tank

Contents

| | |
|---|----|
| 1. Introduction | 4 |
| 2. Unpacking | 6 |
| 3. Safety advice | 8 |
| 4. Installation and start-up | 9 |
| 5. Programming | 18 |
| 6. Running a sterilization cycle | 24 |
| 7. Maintenance | 38 |
| 8. Troubleshooting, alarms and messages | 47 |
| 9. Recycling and disposal | 55 |

ANNEXES

| | |
|--|----|
| 1 Technical data | 56 |
| 2 Maintenance of dental handpieces | 57 |
| 3 Sterilization load preparation | 58 |
| 4 Bowie & Dick test | 60 |
| 5 Helix test | 61 |
| 6 Vacuum test | 62 |
| 7 Water quality | 63 |
| 8 Example of a cycle data report | 64 |
| 9 Accessories and spare parts | 65 |
| 10 Helix test documentation form | 71 |
| 11 W&H Installation check-list | 72 |

1. Introduction



About this manual

This manual contains the Instructions for Use of the W&H sterilizers LINA PR013-003-17 and LINA PR013-003-22, hereinafter referred to as LINA 17 and LINA 22.

All drawings, images and texts contained in this manual are the property of the manufacturer.

All rights reserved. Even partial duplication of drawings, images or text is prohibited.

The information contained in this document is subject to change without prior notice.



For your safety and the safety of your patients

The purpose of this manual is to provide you with information about LINA sterilizers to ensure:

- proper installation and set-up;
- optimal use;
- safe and reliable operation;
- compliance with regular maintenance and servicing requirements.



Please carefully read the safety information in Chapter 3!

Intended use of the product

Small steam sterilizers are widely used for medical purposes, e.g. in general medical practices, dentistry, facilities for personal hygiene and beauty care and also veterinary practices. They are also used for materials and equipment, which are likely to come into contact with blood or body fluids, e.g. implements used by beauty therapists, tattooists, body piercers and hairdressers.

The devices is intended for professional use only by trained people.



Responsibility of the manufacturer

The manufacturer can only accept responsibility for the safety, reliability and performance of the product when the product itself is installed, used and serviced in accordance with the instructions for use.

Servicing by unauthorized persons invalidates all claims under warranty and any other claims.


Introduction


Qualifications of the users

There are two types of users who may operate the sterilizer:

- **The Advanced user** is the head of the clinic/practice, who is legally responsible for the efficiency of the hygiene protocol in place as well as the sterilization process. He/she is also responsible for the USERS' training and the correct operation and maintenance of the equipment.
- **The Users** are the persons who use the sterilizer according to the ADVANCED USER's instructions. They must be trained in operating the sterilizer and in its safe use. Training must be regular and evidence of the understanding shall be recorded.

Conformity to European Standards and Directives

 **0051** Medical Device Directive 93/42/EEC for devices class IIb, in accordance with the Rule 15 – ANNEX IX of the Directive.

 **0497** Directive PED 2014/68/EU (Pressure Equipment Directive) for every sterilization chamber designed and manufactured in conformity to the ANNEX 1 and to the procedure described in the module D1 Annex III.



Directive 2012/19/EU (WEEE) for disposal of parts coming from electrical or electronic products.

IEC 61010-1: Safety requirements for electrical equipment for measurement, control and laboratory use, general requirements


IEC 61010-2-40: Safety requirements for electrical equipment for measurement, control and laboratory use; particular requirements for sterilizers and washer-disinfectors used to treat medical materials.

IEC 61326-1: Electrical equipment for measurement, control and laboratory use; EMC requirements, general requirements.



See the Declaration of Conformity and the Warranty Card in the enclosed documents.

2. Unpacking

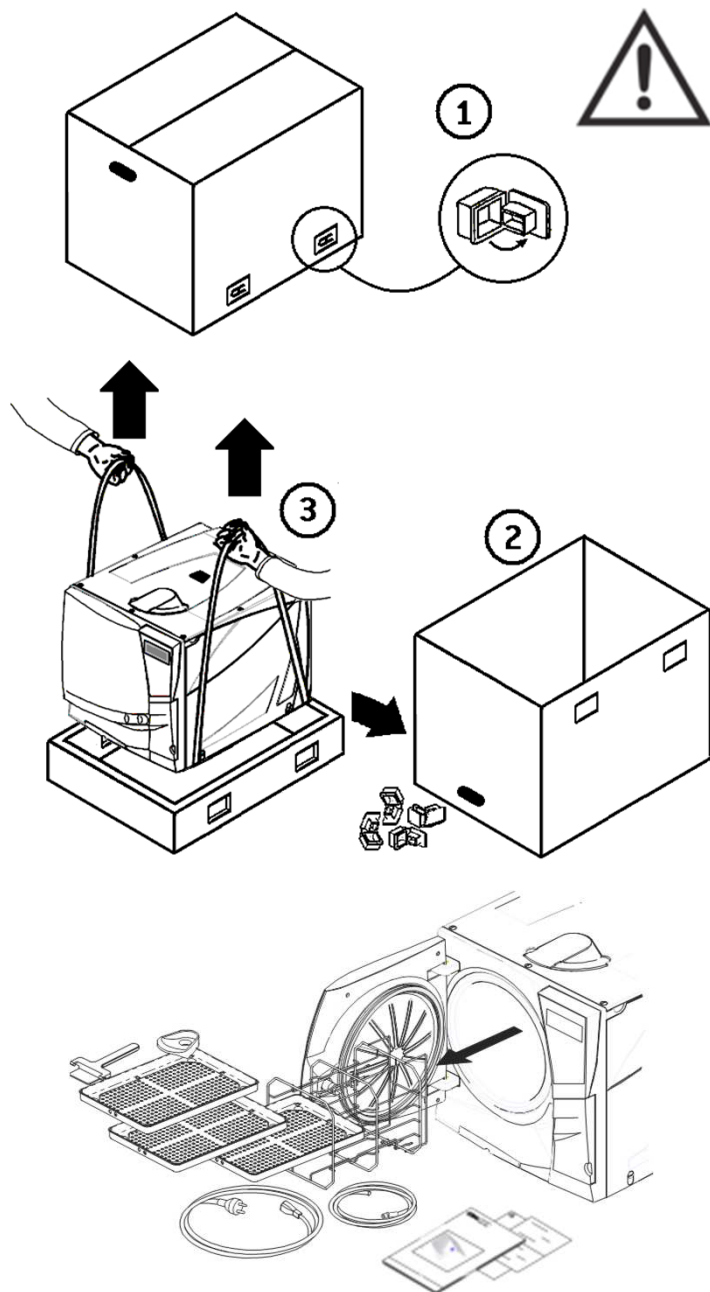

If the sterilizer comes from a cold location, wait until all external and internal surfaces are free from moisture before switching it ON.

The sterilizer must be removed from the box and transported by two people.

Weight: LINA 17: 39 kg

LINA 22: 40 kg

Check the external conditions of the box and the sterilizer. In case of any damage, immediately contact your dealer or the shipping agent that has carried out the transport.



The packaging of the product is environmentally friendly and can be disposed of by industrial recycling companies.



However, we recommend to keep the original packaging should you ever have to ship or transport the sterilizer.

To unpack the sterilizer:


- 1) Open the four locks with your finger and remove them;
- 2) Lift the cardboard top box;
- 3) Remove the sterilizer from the basement using the belt provided.

All accessories are in the sterilization chamber.


Open the front door.

Remove all items except the trays and the tray rack.


Contents of the package

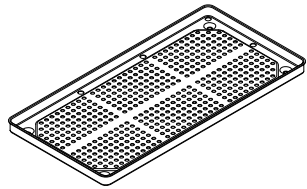


Tray (3 pieces total)




Reversible rack




USB pen Drive loaded with Instructions for use




Tray holder

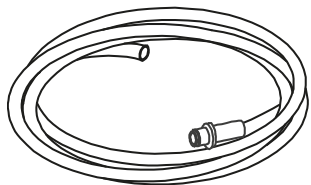


Drain tube

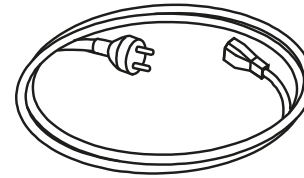


Mains cable




Funnel



Wall spacer

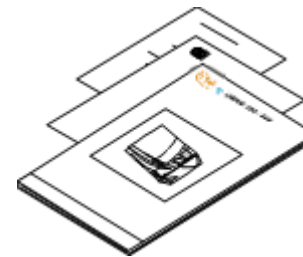

Fast guide
Declaration of conformity
Warranty card
Works tests report
 Maintenance sheet

3. Safety advice



- The product is intended for indoor use only.
- The user is responsible for the proper installation, the correct use and maintenance of the sterilizer in accordance with the instructions listed in this manual.
- The sterilizer has not been designed for the sterilization of foodstuff or waste.
- The sterilizer must not be used in presence of explosive or flammable gases, vapours, liquids or solids.
- The chamber is automatically heated up to high temperature as soon as the sterilizer is switched on – risk of burns!
- Ensure that the socket the mains cable is connected to is properly grounded.
- The trays and the sterilization load will be hot at the end of each cycle. Use tray or cassette holders to empty the sterilization chamber.
- Do not exceed the maximum load weight limits as specified in this manual (see Chapter 6).
- Do not remove the name plate or any label from the sterilizer.
- To avoid electrical short circuits, do not pour water or any other liquids over the sterilizer.
- Use only the power cord set provided by the manufacturer.
- Switch off the sterilizer and unplug the mains cable before inspecting, carrying out maintenance or servicing the sterilizer.
- All electric devices connected to the sterilizer shall be of Insulation Class II (double insulated) or higher.
- If the sterilizer is connected to a water supply system, this must be fitted with a backflow preventing device complying to IEC 61770.
- Repairs, maintenance or service must be carried out by service technicians authorized by the manufacturer and using genuine spare parts only.
- In case of transport:
 - Completely drain both water tanks (see section “Water Tanks” in Chapter 4).
 - Allow the sterilization chamber to cool down.
 - Use original or appropriate packaging.

4. Installation and start-up



Placement

Place the sterilizer on a flat and level surface, far from sources of heat and from flammable materials. Do not place the sterilizer so that it is difficult to open the service door and operate on the controls in it. Do not place the sterilizer so that it is difficult to disconnect the power supply plug. Place the sterilizer in a well-ventilated room. If installed in a cabinet, this shall be provided with an opening of at least 200x150 mm on the rear side. The sterilizer must not be operated in presence of explosive atmospheres.

Required minimum clearances

| | |
|-----------------------|---|
| Back side: | 50 mm |
| Right and left sides: | 10 mm |
| Upper side: | As required for filling the water tank, 50 mm minimum |

Electrical connection


The electrical power supply to the sterilizer must fulfil all applicable standards in the country of use, and must comply with the data label on the back of the sterilizer. Use only the cord set provided by the manufacturer.



Connect the cord set to the socket provided in the back of the sterilizer.

Connect the mains cable to a wall outlet with the following characteristics:


- Single - phase 200 - 240 V, 50/60 Hz - 10A, on a dedicated circuit;
- Overvoltage category = II;
- Protected by a suitable circuit breaker and a residual-current device. All protection devices must be certified according to applicable standards;
- Maximum current absorbed by the sterilizer: 10A;
- A grounded connection is essential.

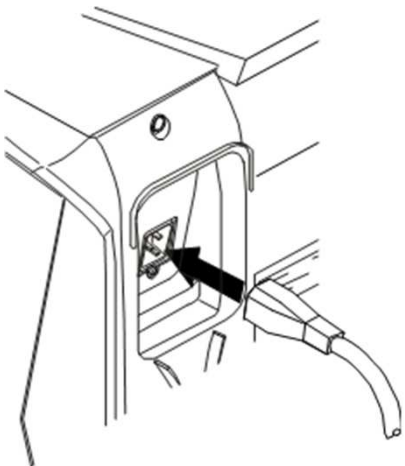

Water tanks

Filling the clean water tank

- Switch the sterilizer ON
- Slide the tank cover to the right to access the clean water tank inlet.
- Remove the cap from the tank inlet;
- Insert the funnel and fill the water tank with approx. 4 litres of distilled or demineralized water;
- Once the clean water tank is almost full, an audible tone will sound; stop filling;
- Place the cap to close the tank;
- Slide the tank cover back into its original position.

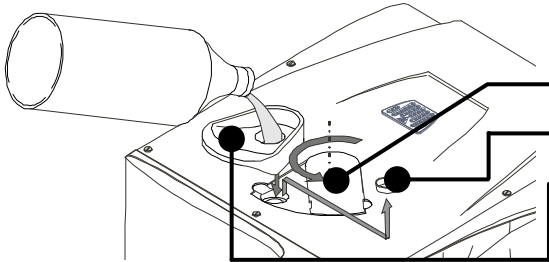




Do not use tap water to fill the clean water tank

Use only distilled or demineralized water as described in ANNEX 7.

Do not add any chemical / additive to the water.

Draining the used and clean water tank



- Open the service door at the front of the sterilizer.
- Put a container (4 litres min) below the sterilizer and insert into it the free end of the drain tube.
- Insert the drain tube into the left connector (grey) for the used water, or into the right connector (blue) for the clean water.
- Let the water flow from the tank completely.
- Press the push-button on top of the quick connector to dislodge the drain tube.

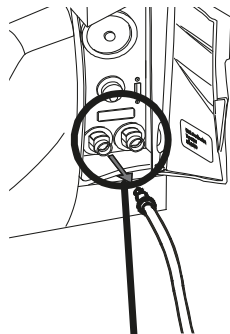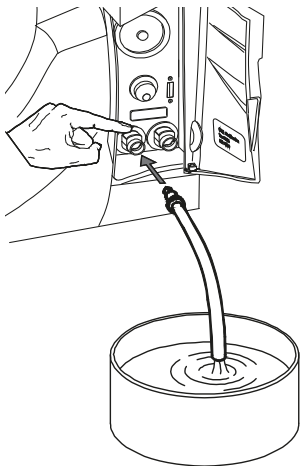

Used water drain (grey)


Clean water drain (blue)

Chamber furniture

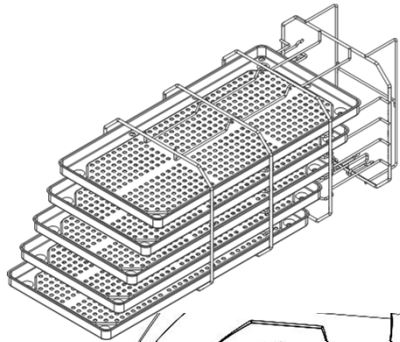

Before touching the chamber furniture, ensure the sterilization chamber is cold: risk of burns!

The chamber furniture consists of the **trays**, the **tray rack** and the **steam diffuser plate**.

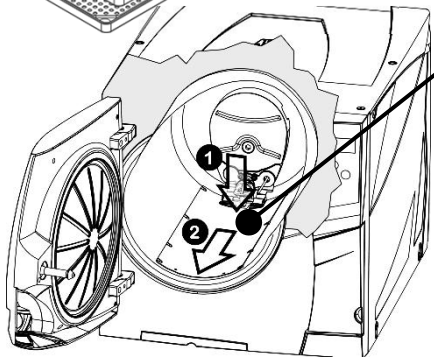


Steam diffuser plate



Ensure that the steam diffuser plate is firmly hooked in its position before starting a sterilization cycle. An improper positioning of the steam diffuser plate could result in bad steam quality and could impair the sterilization process, with risk of non sterile load and cross infection.

Sterility at the end of the cycle is not guaranteed if the steam diffuser plate was not correctly placed. **To hook** the steam diffuser plate, slide it into the chamber until it gets engaged into the end hooks. **To remove** the steam diffuser plate, press it in the center of the end edge (1) and slide it outwards (2).

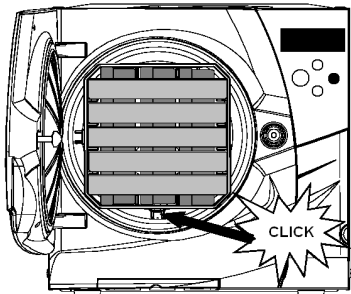


Tray rack

Insert the rack into the sterilizer chamber, align it at the center/bottom of the chamber and push it gently into position until it clicks.

The chamber rack is reversible and can accommodate 5 trays horizontally or 3 cassettes vertically.

If inserted in a 90° degree rotated position, the rack holds 3 trays or 3 cassettes horizontally.

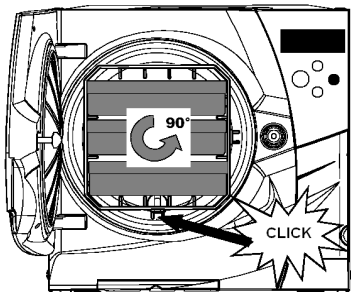


Usable space in the chamber

LINA 17: 195 x 195 x 297 mm (WxHxD); equal to the volume of 11.5 litres.


LINA 22: 195 x 195 x 390 mm (WxHxD); equal to the volume of 15 litres.

Controls, commands, connections

Front view

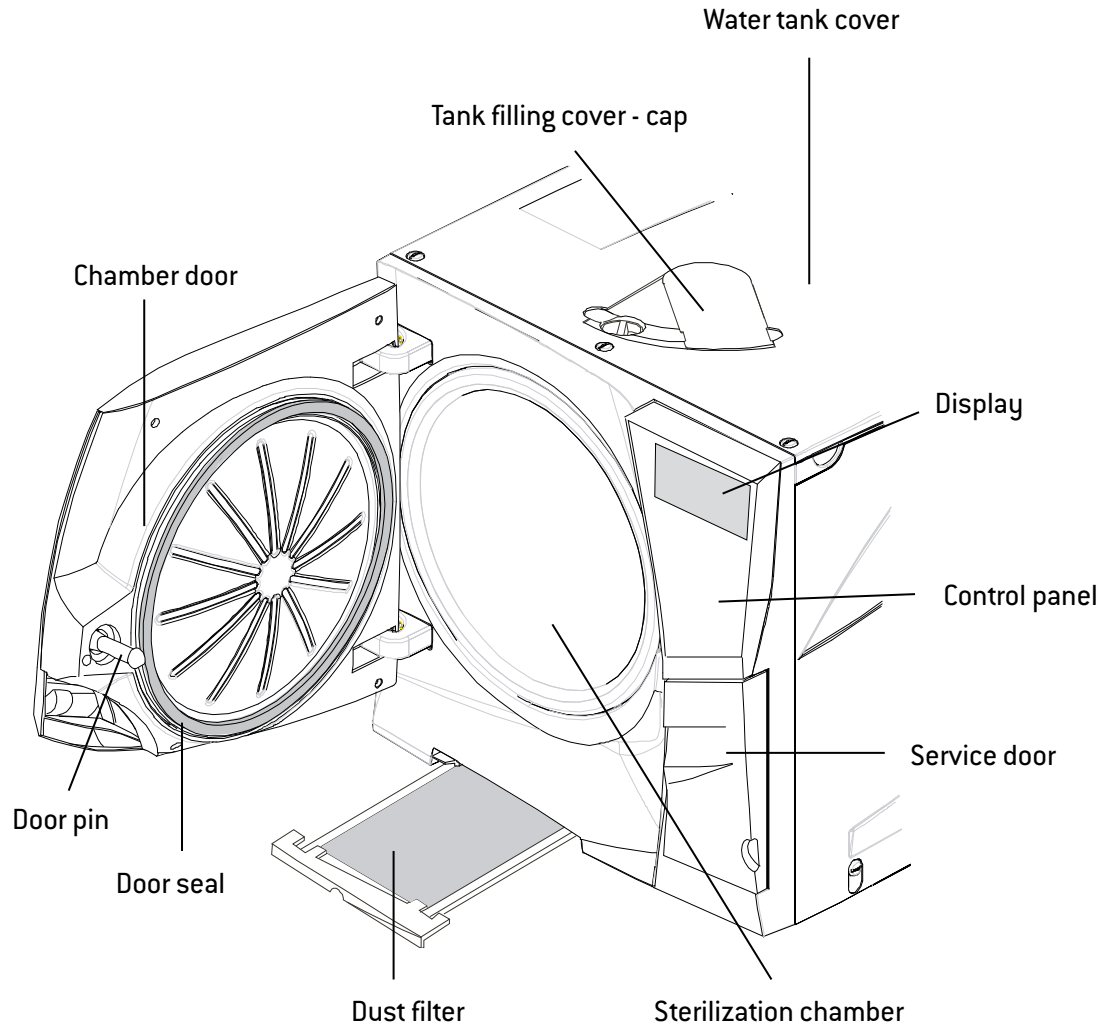

Service door

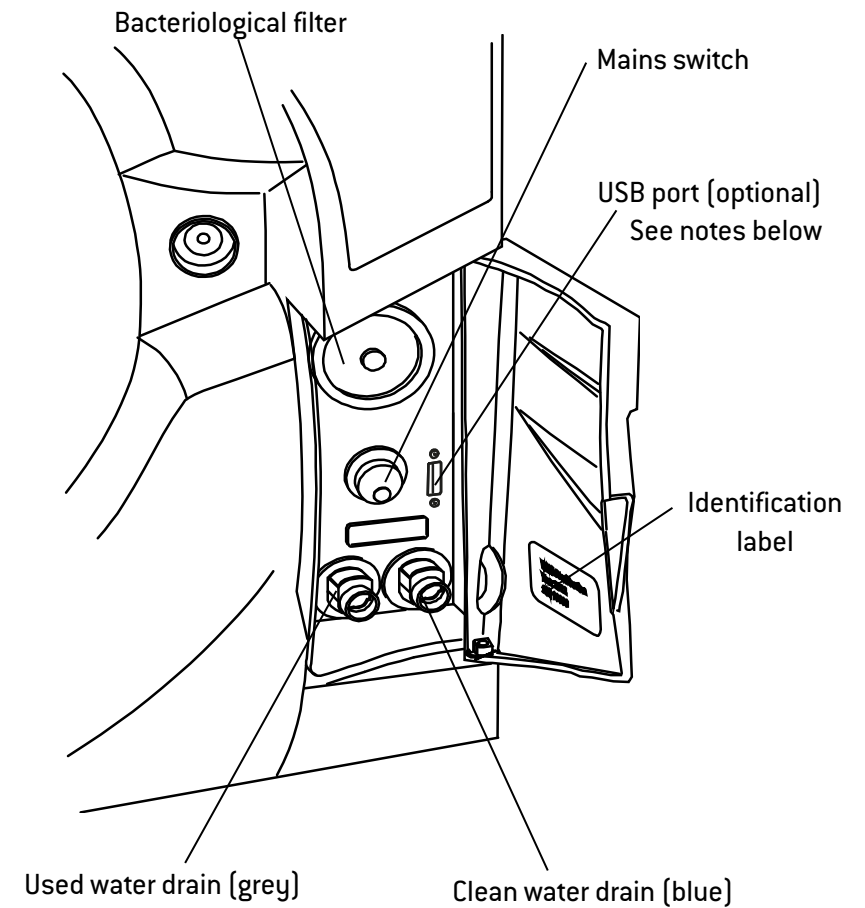


Keep the USB pen drive provided plugged into the USB port, so that all sterilization cycle reports will be saved in it.




To prevent data loss or corruption, periodically copy the whole data in the USB pen drive to a computer or to another safe support.

Connections

Rear view

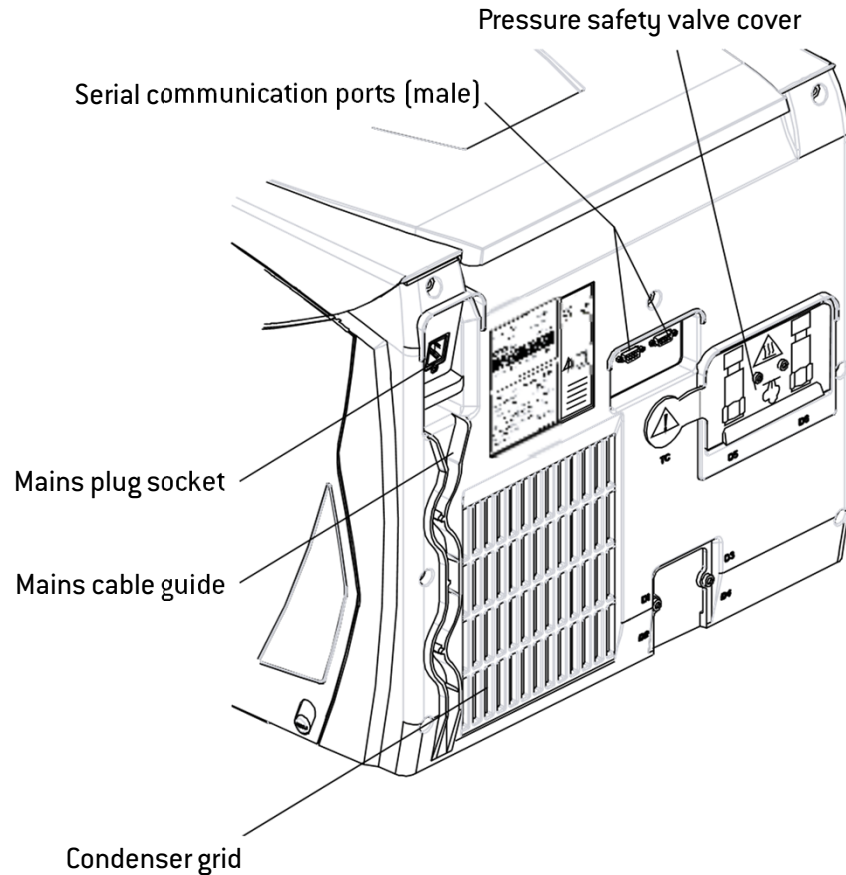

Detail of the hydraulic connections (optional)

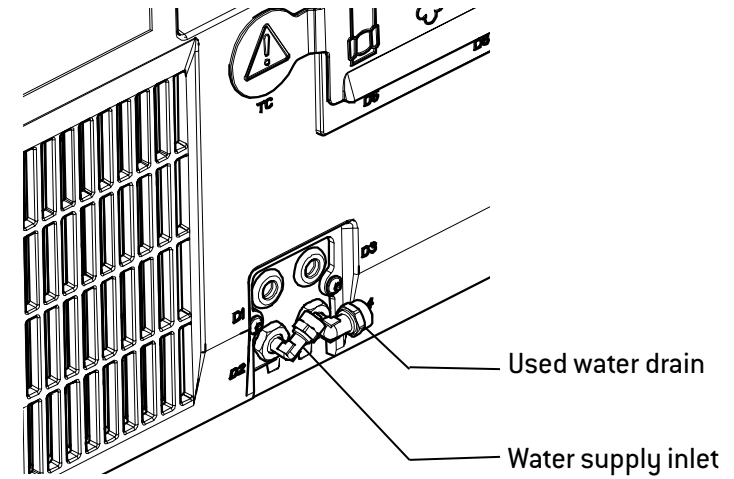

All cables and tubes connected on the rear side of the sterilizer must be placed far from the condenser grid (e.g. using the available guides).



The water supply system must deliver demineralized water meeting the requirements as listed in ANNEX 7.

Do not add any chemical / additive to the water.

The manufacturer's warranty is void if the sterilizer was used with water containing either chemical additives, or contaminant levels exceeding those listed in ANNEX 7.




The water supply system must be fitted with a backflow preventing device complying to IEC 61770 and to national and local regulations.



The maintenance of the external water filling system must be done in exact accordance with the information of the instructions for use given with the relevant system.

Controls and commands

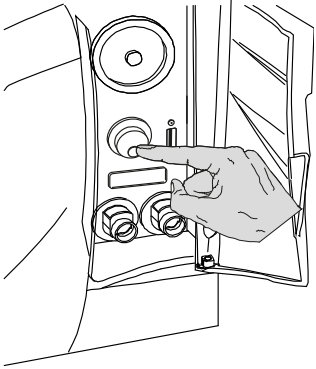

Switching ON the sterilizer

Press the mains switch behind the service door to switch ON the sterilizer.

The visual indicator on the mains switch turns green and the START screen (see next page) appears.


“SLEEP” mode

In “SLEEP” mode the display remains dark and the sterilizer chamber is no longer heated to save energy.

If the sterilizer is not used for 12 hours, (the time interval can be changed, see Chapter 5 - Programming) it will automatically switch to “SLEEP” mode.

Exit from “SLEEP” mode through any of the following actions:

- Press any button on the control panel;
- Open or (if it is open) close the chamber door.

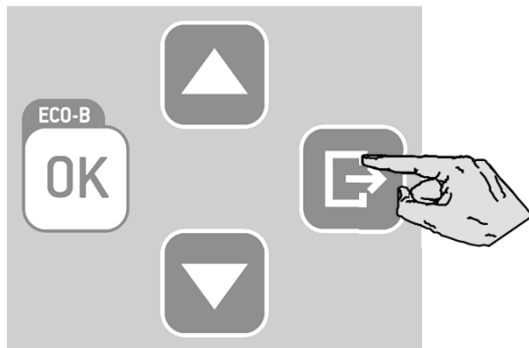

It is also possible to put the sterilizer into “SLEEP” mode manually:

On the START screen, press the BACK button.

A 10 second countdown will commence. At the end of the countdown the sterilizer will enter the “SLEEP” mode.

The countdown can be stopped at any time by pressing the BACK button.

Display and icons

First line


Shows the title/purpose of the current page and invites you to take an action (e.g. select a cycle).

Second line

Shows the active option/action (preceded by the cursor \rightarrow).
By pressing OK, the active option/action will be selected/executed.
Pressing UP or DOWN changes the active option/action.

Warning, tank and printer icons

The cursor (\rightarrow) preceding an icon means that an information message is to be read.

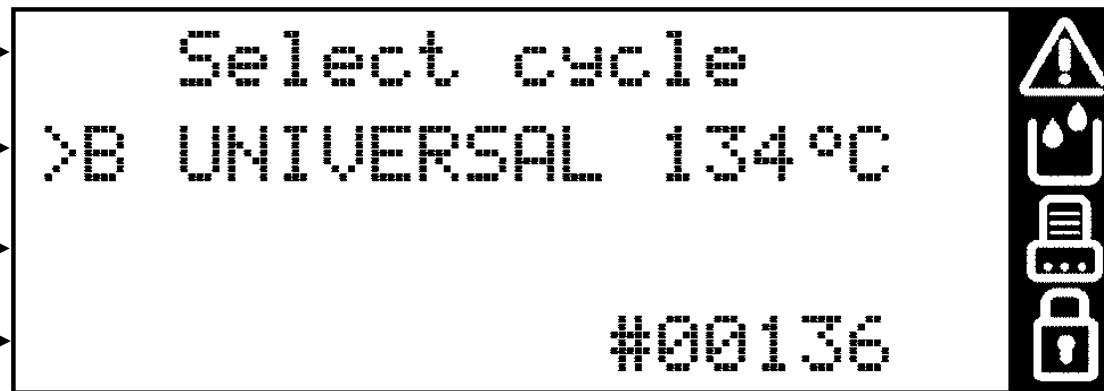

Third and fourth lines

Show additional information about the active option/action.

"Padlock" icon

The cursor (\rightarrow) preceding this icon informs that the door is safely locked.

Icons

If one or more icons of the display are preceded by the cursor, please take the actions as outlined below:



If an icon is preceded by the cursor, this means that an information message is present in the MESSAGES menu. Follow the instructions provided in Chapter 8 to read the relevant messages.



General warning

One or more messages require your attention, or an action is required (e.g. maintenance).



Tank warning

The clean water tank needs to be filled, or the used water tank has to be drained, or a message about the water quality is present.



Printer

An external device (printer, PC, etc.) is not working properly, or is OFF, or is disconnected from the sterilizer.



Door locked

The door is locked. During a sterilization cycle this does not indicate any anomaly.

Control buttons

The control panel shows four buttons:

UP button


Moves to the upper item in the list.
Increases a number or a parameter.

ECO-B option

This label reminds you that, when starting a cycle, you can choose the ECO-B mode by holding the OK button for 2 seconds (see Chapter 6).

OK button (confirmation button)

Confirms the active option.
Confirms a number or a date.
Saves a configuration or a parameter.

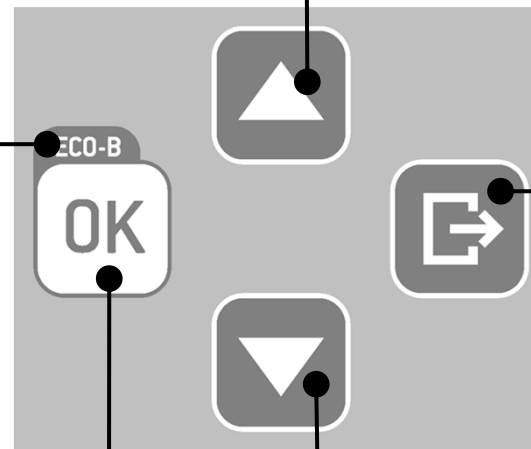

BACK button

Aborts the action/function.
Moves to the previous screen
without confirming/making any
changes nor saving any parameters.


DOWN button

Moves to the lower item in the list.
Reduces/decreases a number or a parameter.

5. Programming

Initial setup

Before using the sterilizer please program important parameters such as date, time, language, display backlight and contrast. This is done by means of the SETUP functions.

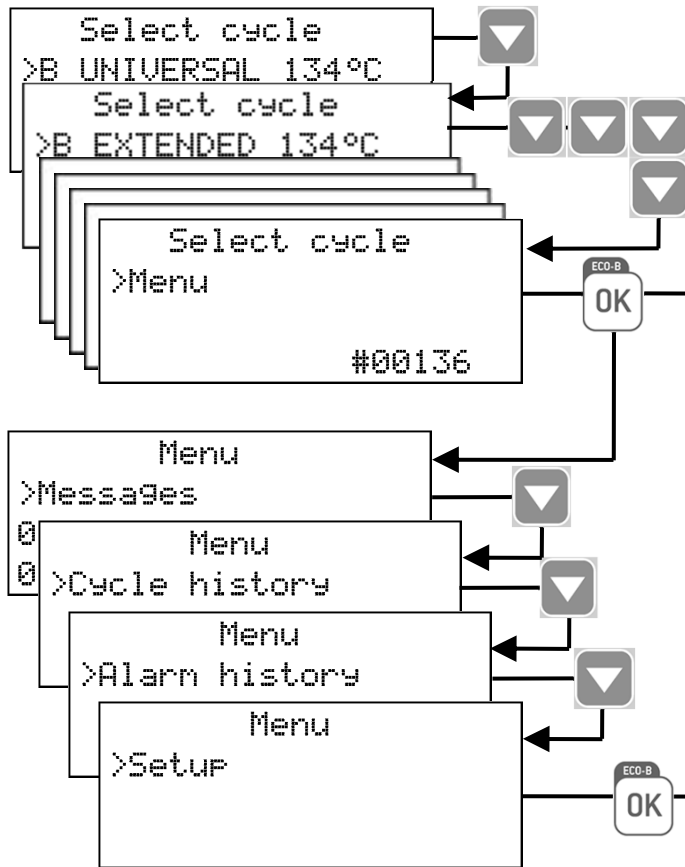

Start screen and menu options

When the sterilizer is switched ON, or when exiting from SLEEP mode, the default cycle program is displayed, preceded by the cursor.

By pressing DOWN the other available cycle programs are displayed. Continuously press DOWN until the MENU option appears.

Menu

Confirm (OK) the MENU option to access all sub-menus and navigate through sub-menus with the UP and DOWN buttons.

See the following pages for a complete description of the options available and how to use them.

Setup

Scroll (DOWN) to SETUP and confirm (OK) to access and set the main parameters of the sterilizer.

See the following pages for a complete description of the parameters you can set and how to do it.

Table 1: list of the MENU options

| MENU | SUB-MENU | WHAT IT DOES | | | |
|--------------------------------------|---------------|--|--|-----|---|
| Menu (continues on next page) | Messages | - | Displays pending messages. Refer to Chapter 8 for a detailed list of messages. | | |
| | Cycle history | Select | Select a previously recorded cycle. Press OK and then scroll the list of the recorded cycles with UP/DOWN. Press OK to select the cycle to be viewed or printed. | | |
| | | View | Displays the selected cycle. Press UP/DOWN to scroll the cycle report. | | |
| | | Print (*) | Prints the selected cycle. Press OK and scroll UP and DOWN to change the number of copies to be printed. Once the value is displayed, press OK to print. | | |
| | | Print labels (*) | Prints traceability labels for the selected cycle. Press OK and scroll UP and DOWN to change the number of copies to be printed. Once the value is displayed, press OK to print. | | |
| | | Save HTML (*) | Saves a cycle data file on the USB mass storage device | | |
| | | Send HTML (*) | Sends a cycle data file to the serial port for storage on an external device (e.g. a PC). | | |
| | Alarm history | View alarms | Displays all the alarms that have occurred during sterilization cycles. | | |
| | | Print all (*) | Prints all the alarms that have occurred of the sterilization cycles stored in memory. | | |
| | Setup | Sets important parameters of the sterilizer such as date, time, language, etc. Confirm [OK] to access all available options. Refer to TABLE 2 for a detailed list of options and related programming. | | | |
| | Configuration | Aut. water supply | Enables the automatic water feed | Yes | Press UP/DOWN to scroll the YES/NO options, then press OK to enable/disable the function (warning), or BACK to exit without saving. |
| | | Ext. water sensor | Enables water quality warnings based on the external/internal sensor | No | |
| | | Int. water sensor (*) | | | |
| | Service | Current level | Allows the user to change the current user level. Access to ADVANCED USER level or SERVICE level is protected by codes. See “How to log in as an advanced user” in the following pages. | | |
| | | Activation code | Allows the user to enter the activation code in order to enable some optional features. | | |

(*) available/effective only if a suitable endorsed device (printer, logger, PC, water supply, etc.) is connected and enabled in the SETUP menu.

Table 1: list of the MENU options (continued)

| MENU | SUB-MENU | WHAT IT DOES | | |
|---|---|---------------------|---|--|
| Menu (continued from previous page) | Print lot labels (*) | Print | Prints traceability labels to be stuck to the load pouches. Labels show the lot number and other parameters as specified in the LOT LABELS menu (see SETUP table). The number of labels will be requested: press UP/DOWN to increment/decrement the number, then press OK to print. After printing, the lot number is incremented by 1. | |
| | | Reprint | Prints labels of a previous sterilization lot. The lot number and the number of labels will be requested: press UP/DOWN to increment/decrement the numbers, then press OK to print. | |
| | Device info | Brand | Displays the device brand name; e.g. W&H. | |
| | | Model | Displays the device model name; e.g. LINA. | |
| | | Type | Displays the device type; e.g. PR013-003-22. | |
| | | Serial number | Displays the serial number of the sterilizer; e.g. 110009. | |
| | | Performed cycles | Displays the total number of cycles executed by the sterilizer. | |
| | | Service counters | Dust filter | Displays the status (number of cycles executed) of consumables. Permits the user to reset the counter to zero after replacing a consumable. See Chapter 7 (Maintenance) for details. |
| | | | Bac. filter | |
| | | | Door seal | |
| | | | 4000 service | Displays the number of cycles executed compared to the 4000 cycle service. |
| | | Software rev. | Displays the current software version. | |
| | | Boot version | Displays the current system software version. | |
| | | Power version | Displays the current version of the power firmware. | |
| | | USB4 Soft. rev. | Displays the current version of the USB4 software | |
| USB4 Boot rev. | Displays the current version of the USB4 system software | | | |
| Format | Formats the USB4 device (pen drive) WARNING! All data in will be erased! | | | |
| HW key ID | Shows the identifier of the hardware key (label printer/service), if connected. | | | |
| PC/logger port | Displays the port to which the PC/logger device is connected. | | | |
| PC/logger version | Displays the software version of the PC/logger device, if connected. | | | |

(* available/effective only if a suitable label printer is connected and enabled in the SETUP menu.

Table 2: Detail of the SETUP options

| MENU | SUB-MENU | | WHAT IT DOES AND HOW TO SET IT | | |
|-----------------------------------|------------------|---|---|---|--|
| Setup (continues on next page) | Language | Sets the language. The active language is displayed: press OK and scroll other available languages with UP or DOWN. When the new language is displayed press OK to confirm, or BACK to exit without saving. | | | |
| | Date and time | Set date and time | Sets the time and date which will be used for the cycle report and for the delayed cycle start option. By pressing OK the cursor is positioned on the date. Change the month, year and the day with UP or DOWN. By pressing OK, the changes are saved and the cursor moves to the time setting. The procedure for setting the time is the same. During the procedure, you can press BACK to return to the SETUP menu without saving. | | |
| | | Date format | Sets the date and time display formats. Press OK to access the function and then scroll with UP and DOWN until the preferred format is displayed. Press OK to confirm. Press BACK to exit without saving. | | |
| | | Time format | | | |
| | User name | Sets the operator or dental clinic name which will be used for the cycle report. There are 18 characters (capital letters and numbers) plus space, the dash and the point. You can store only one name. By pressing OK the saved name is displayed, or a series of dashes if no name is saved. Press UP and DOWN to change characters. Press OK to save a character and the cursor will move to the next character. To return to the previous character, press BACK. To go to the next character without changing it, just press OK without pressing either UP or DOWN. To go to the last character hold OK for two seconds. Press BACK on the first character to exit without saving. Press OK on the last character to save the name as displayed. | | | |
| | Sleep mode | Sets the time before the sterilizer will enter "SLEEP" mode. In "SLEEP" mode the sterilizer consumes less energy. It is advised to set a short "SLEEP" mode time in order to save energy. See Chapter 4 "CONTROLS AND COMMANDS" for a description of "SLEEP" mode. Press OK to view the current time. Press UP or DOWN to increase or decrease the time by increments of 10 minutes from 10 minutes to 12 hours. Press OK to save the time. Press BACK to exit without saving. | | | |
| | Volume setting | Increases or decreases the sound volume. Press OK to view the current setting. To decrease or increase the volume press UP or DOWN: a sound will be emitted as an example. Press OK to save the new setting. Press BACK to exit without saving. | | | |
| | Display contrast | Sets the display contrast. Press OK to view the current setting. Press UP to increase or DOWN to decrease the contrast. Press OK to save the new setting, or BACK to exit without saving. | | | |
| | Serial port | Sets the device that is connected to the serial port. (not available if the USB kit is installed) | | Not used | Serial port not in use. |
| | | | | Printer | Serial port used for cycle report printer. |
| Label printer | | | | Serial port used for label printer (available only if a label printer is present and configured). | |
| PC/logger | | | | Serial port used for an external PC/LOGGER (see APPENDIX 9 – Accessories). | |
| Label printer | Model | Sets the label printer model See note (*) for instructions | | | |
| | Offsets | Horizontal offset | Set the horizontal and vertical offsets of the label layout. Adjust the values according to note (*) , until the printout is properly centred in the label | | |
| | | Vertical offset | | | |

Table 2: Detail of the SETUP options (continued)

| MENU | SUB-MENU | WHAT IT DOES AND HOW TO SET IT | | |
|---|------------------------|--|---|---|
| Setup (continued from previous page) | Printer [S2] | Sets the printer model | See note (*) for instructions. | |
| | Preheating (**) | Sets the preheating mode See note (*) for instructions | Door closed | Preheats the chamber ONLY if the chamber door is closed. |
| | | | Never | Chamber is never preheated. |
| | Hot surf. warning (**) | Sets the warning See note (*) for instructions | Yes | A warning appears while the door is open and the chamber hot. |
| | | | No | No warning appears. |
| | PC/logger warning (**) | Sets the warning See note (*) for instructions | Yes | A warning appears if the PC/LOGGER is not detected or if data saving fails. |
| | | | No | No warning appears. |
| | Units (**) | Pressure | Sets the unit for pressure | See note (*) for instructions. |
| | | Temperature | Sets the unit for temperature | |
| | Traceability | Cycle reports | Save HTML | Enables automatic saving of the cycle report on the USB device (****) |
| | | | Autom. printing (***) | Enables automatic printing of the cycle report. |
| | | | SCL saving | Enables saving of a complete data set of parameters each second (takes more memory space) |
| | | | HTM2010 option | Enables printing the plateau temperature at fixed time steps (use the next option to set the step). |
| | | | HTM2010 step | Sets the time step |
| | | Cycle labels (***) | Autom. printing | Sets the number of labels to be printed automatically at the end of each successful sterilization cycle. |
| Manual printing | | | The user will be asked for the number of labels to be printed at the end of each successful sterilization cycle. Press UP/DOWN to increase/decrease, OK to confirm. Press BACK to exit without printing. | |
| Expiry time | | | Sets the expiry time (in weeks) for labels. The software will automatically add the programmed expiry time to the current date and print it on labels. If it is set to zero, no expiry date will be printed on labels. | |
| Lot labels (***) | | Set counter | Sets the lot number to be printed on the labels (it will be increased at each lot). | |
| | | Label fields | User name | Sets the information (user name, time/date, expiry date) to be printed on the labels. |
| | Date and time | | | |
| Expiry time | | | | |

Note (*) The current setting is displayed: press OK to enable changes and then UP/DOWN to scroll the available options. Press OK to set a new option, or BACK to exit without saving.

Note ()** This option is available for advanced users only. See the next page for instructions about how to log in as an advanced user.

Note (*)** This option is available only if a compatible label printer is connected.



Note (**)** It is strongly recommended to periodically backup the data from the USB drive to a safe support.

How to log on as an advanced user

Some programmable options of the LINA sterilizer can be changed only after logging in as an advanced user.

This is to prevent accidental changes or unexpected operation of the sterilizer.

Hiding a cycle program, making it inaccessible to users, is an example of option that can be accessed by advanced users only.

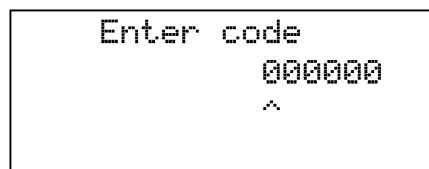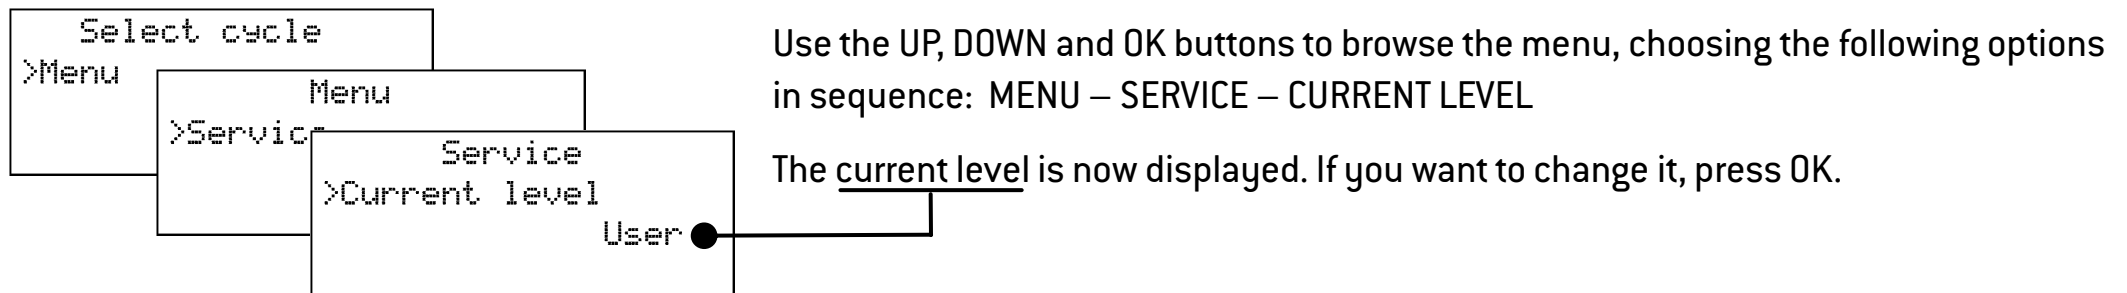

The screen as shown to the left will appear: you can now type in the advanced user code (000123) using the UP, DOWN, BACK and OK buttons as follows:


- UP/DOWN to increase/decrease the current number (indicated by the cursor `■`);
- OK to save the number and move to the next one;
- BACK to move to the previous number.

Press OK on the LAST number to confirm the code .

Press BACK on the FIRST number to abort the procedure.

After making the desired changes in the advanced user level, return to the user level by setting all numbers to zero, or switch OFF the sterilizer and then ON again.

6. Running a sterilization cycle



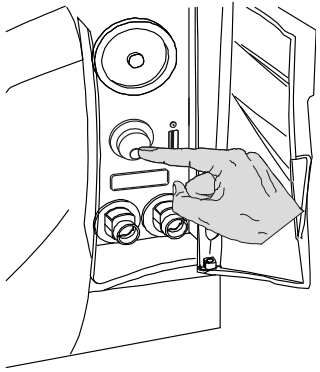


Place the sterilization load in the sterilizer chamber and close the door.



See ANNEXES 2 and 3 on how to properly prepare and place the load.

Switch the sterilizer ON by pressing the mains switch behind the service door.

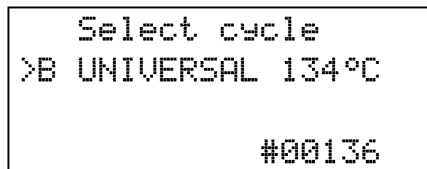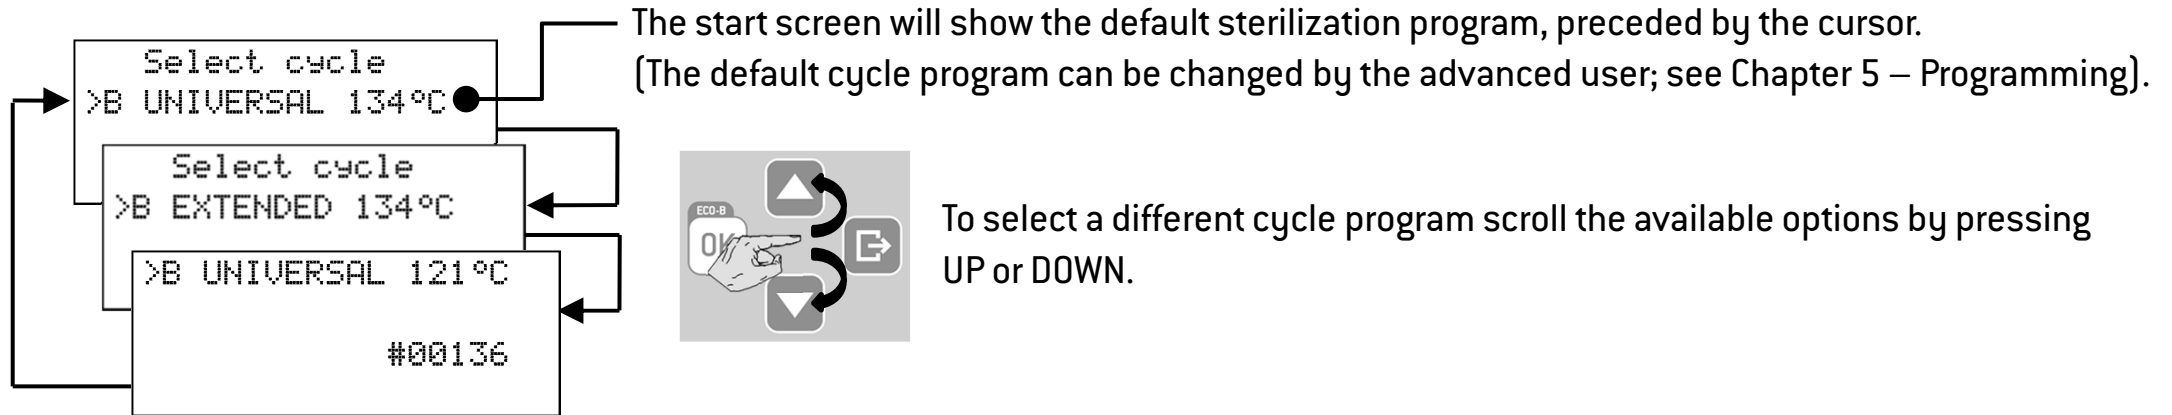

Select the desired cycle program by pressing OK.



To start the cycle in ECO mode, hold the button for 2 seconds (see page “The ECO-B option in this Chapter”).

Running a sterilization cycle

After selecting the cycle:

- the first line of the display shows the selected cycle.
- the "START NOW" option appears: press OK to start the sterilization cycle immediately, otherwise see the next pages for the "delayed start" options.
- the third and fourth lines show the maximum load weight limits for the selected cycle.
- if you want to select a different cycle, press BACK to return to the cycle selection screen (see previous page).

```
B UNIVERSAL 134°C
>Start now
Max. 5kg instr.
Max. 1.8kg textile
```

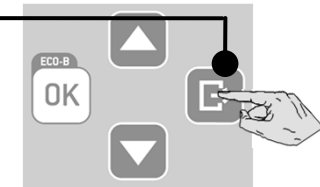

After initiating the cycle:

- the door locks automatically (the cursor appears near the "padlock" icon);
- the sterilization cycle starts;
- the second line shows the approximate residual cycle time;
- the third and fourth lines show the "Cycle-in-progress" information (see "Cycle in progress" in the following pages of this chapter)

```
B UNIVERSAL 134°C
> 42:00
T: 22.5°C PV1
P: 0.00bar #00136 >
```



Emergency during the door locking:

While the door is getting locked, the user may reopen it immediately by pressing any button on the panel. This action is possible during the motor operation and for two seconds more.



See the following pages for a description of each cycle program (temperatures, times, maximum load weights).

The available sterilization cycles

In total there are three sterilization cycles available. All cycles are type B according to the European Standard EN13060, which means they are capable to sterilize all types of loads: full solid, porous, hollow A and B, plastics, rubber, etc.; unwrapped, bagged, single or double wrapped.

Select the **B UNIVERSAL 134°C** cycle for all your general items like hand instruments, handpieces, forceps, etc.

Select the **B EXTENDED 134°C** cycle if a 18 minute sterilization plateau time is required for your load or mandated in your country.

Select the **B UNIVERSAL 121°C** cycle for all items that cannot withstand the high temperatures of the 134 cycles, such as textiles and plastics.

NOTE: In some Countries, the cycle **B EXTENDED 134 °C** is named as **B PRION 134°C**.

Depending on Country requirements, other cycle names might be different too.

For your safety and the safety of your patients



Never exceed the maximum load weight limits as specified in the cycle program table (see next page) as this could impair the sterilization process.

The display reminds the maximum permitted load before starting a cycle

The available sterilization cycles

| | | STERILIZATION CYCLES | | | | | | | | | | | | | |
|--|-------------|--|------|---------|---------------------------------|------|---------|-------------------------|--------------------|--------------------|---|--|---|--|--|
| | | B UNIVERSAL 134°C | | | B EXTENDED 134°C B PRION 134 | | | B UNIVERSAL 121°C | | | B UNIVERSAL 134°C ECO MODE | | B EXTENDED 134°C B PRION 134 ECO MODE | | |
| Sterilization temperature | | 134°C | | | | | | 121°C | | | 134°C | | | | |
| Sterilization pressure | | 3.03 bar 2.03 bar(g) | | | | | | 2.04 bar 1.04 bar(g) | | | 3.03 bar 2.03 bar(g) | | | | |
| Duration of the Sterilization phase | | 3'30" | | | 18' | | | 15' | | | 3'30" | | 18' | | |
| Duration of the drying phase ⁽³⁾ | LINA 17 | 23' | | | | | | 30' | | | 7' | | | | |
| | LINA 22 | 25' | | | | | | 30' | | | 7' | | | | |
| TOTAL CYCLE DURATION ⁽¹⁾ | LOAD | Empty | Full | Typical | Empty | Full | Typical | Empty | Full | Typical | Full | | Full | | |
| | LINA 17 | 40' | 54' | 49' | 55' | 69' | 64' | 60' | 74' ⁽⁴⁾ | 68' ⁽⁴⁾ | 29' | | 44' | | |
| | LINA 22 | 46' | 63' | 55' | 61' | 78' | 70' | 64' | 79' ⁽⁴⁾ | 72' ⁽⁴⁾ | 32' | | 47' | | |
| LOAD TYPE | | All unwrapped, bagged, single/double wrapped instruments: - Solid - Hollow A (Narrow lumen) - Hollow B (Simple hollow item) - Porous | | | | | | | | | All unwrapped, single wrapped instruments: - Solid - Hollow A (Narrow lumen) - Hollow B (Simple hollow item) | | | | |
| MAX. LOAD ⁽²⁾ | LINA 17 | Instruments: 4 kg – porous: 1.5 kg | | | | | | | | | | | | | |
| | LINA 22 | Instruments: 5 kg – porous: 1.8 kg | | | | | | | | | | | | | |
| | | Instruments: 0.5 kg | | | | | | | | | | | | | |

(1) The total cycle time may vary depending on the type of load (solid or porous) and other factors. Values and cycle names could be different depending on country requirements.

(2) The load given includes the trays, the containers and everything is put into the chamber, with the sole exclusion of the tray rack.

(3) The drying time can be increased: see “Customization of cycle parameters” in Chapter 6.

(4) Time specified for textile load.

The available sterilization cycles



For your safety and for the safety of your patients

Never process objects different from those specified in the cycle program table and never exceed the maximum load weight limits specified in it.


Such actions:

- could result in non-sterile conditions at the end of the cycle;
- could expose people to the hazard of cross-infections;
- are considered as an improper use of the sterilizer for which the manufacturer cannot be hold responsible.

All indications of sterile load or successful completion of the cycle that are given on the display at the end of the cycle are not valid if the type and quantity of the load are not complied with.

The sterilization cycle profile

All available sterilization cycles feature the same basic pressure profile as shown in the graph below. The duration of the sterilization phase (or plateau time) and the sterilization temperatures differ between the various cycles.

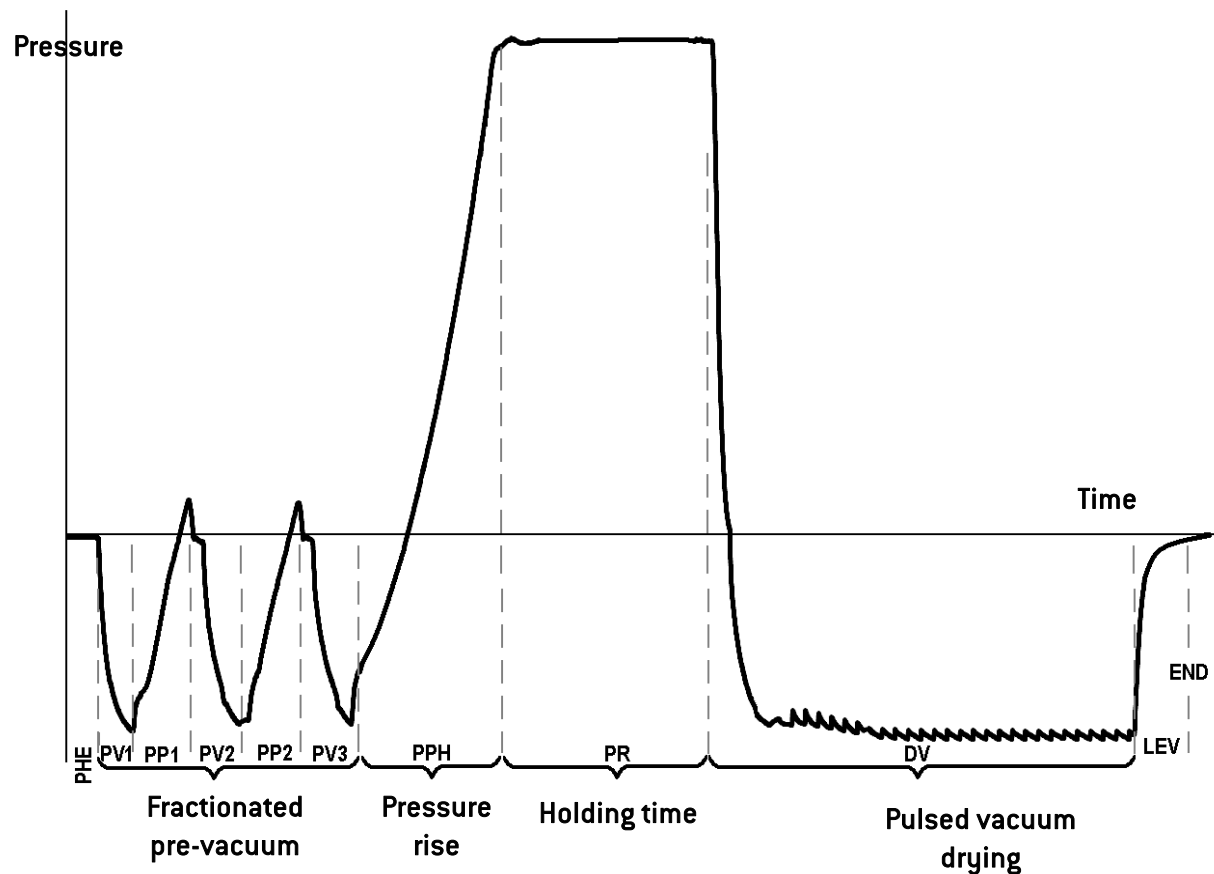


| LEGEND | |
|-----------|--|
| PHE | Pre-heating (this is not considered a part of the cycle) |
| PV1 - PV3 | Vacuum pulse (removal of air from the sterilizer chamber/load) |
| PP1 - PP2 | Pressure pulse (steam generation) |
| PPH | Rise to the sterilization phase |
| PR | Process (holding time) |
| DV | Vacuum drying |
| LEV | Leveling |
| END | End of the cycle |


The ECO-B option

“ECO-B” is a cycle option designed to reduce the cycle duration and the overall energy consumption, providing a fast type B cycle for a limited load weight (0.5 kg of instruments only!).

The “ECO-B” option is available for the B UNIVERSAL 134°C and B EXTENDED 134°C cycles only.

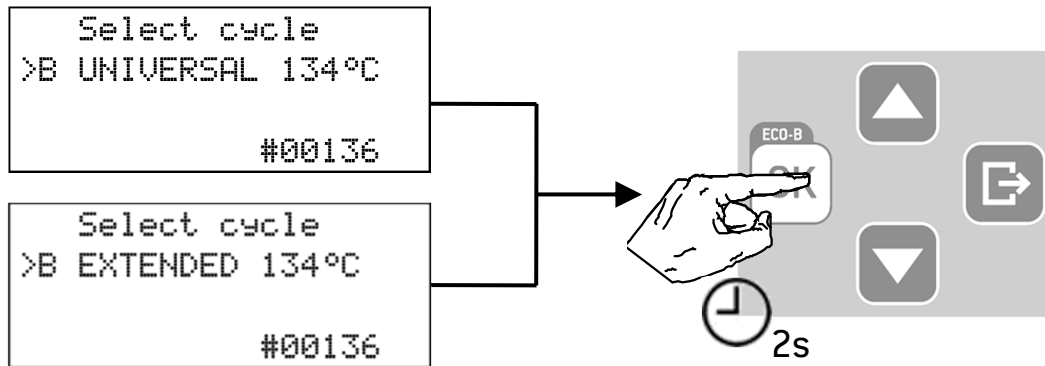

To start a cycle in the ECO-B mode, select the cycle and then confirm your selection by **holding the OK button for two seconds.**

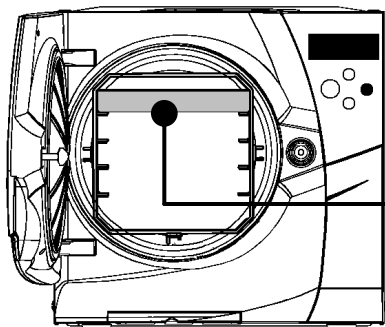

Loading the chamber when running an ECO-B cycle

In ECO-B mode, the maximum load weight limit changes to 0.5 kg of instruments only!


Always place items on the upper tray of the chamber rack and remove all other trays from the chamber. Ensure that the paper side of sterilization bags faces up.



For your safety and the safety of your patients

Never exceed the maximum load weight limits as this could impair the sterilization process.

The “Delayed start” options

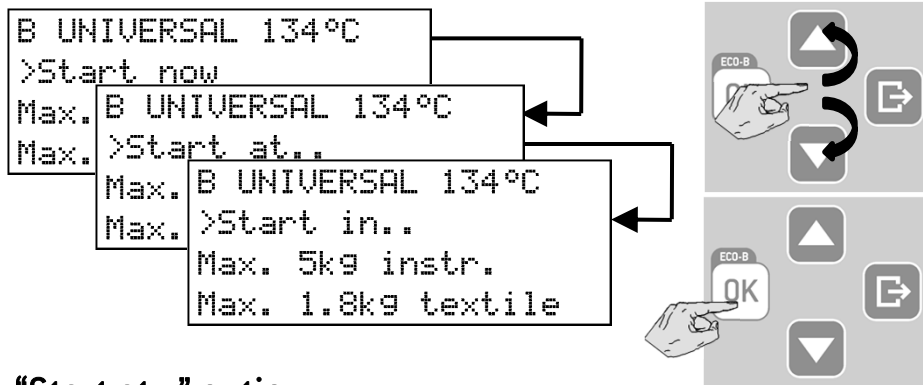

After selecting a cycle program, press UP or DOWN to scroll between the “start now”, “start at...” and “start in...” options.

Select the desired option by pressing OK.



The delayed start option is not available for all cycles.

“Start at...” option

Sets the time and date when the cycle starts.

Press OK: the display shows the last choice. If you accept it press OK, otherwise press UP or DOWN and then OK to select “Set start at...” to set a new time/date: by pressing UP, DOWN and OK you can change the time/date. Press OK to confirm the change. The cycle will start at the indicated time. A countdown timer will appear on the display.

Press BACK at any time to abort the procedure.

“Start in...” option

Sets a waiting interval before the cycle starts by increments of 10 minutes, up to 24 hours.

Press OK: the display shows the last interval used. Press UP or DOWN and then OK to select “Set start in...” to set a new interval.

By pressing UP and DOWN you can change the time interval. Press OK to confirm the change. The cycle will start after the programmed interval. A countdown timer will appear on the display.

Press BACK at any time to abort the procedure.

Stopping the countdown

During the countdown, you can press UP and DOWN to scroll between the two following options:

| | |
|-----------|---|
| Start now | Press OK to stop the countdown and start the cycle immediately |
| Stop | Press OK to stop the countdown and return to the main menu (a further confirmation will be requested) |

Customization of cycle parameters

You can customize a cycle program by setting certain parameters according to your own sterilization protocol.



The drying time can be changed only after acceding as an ADVANCED USER.

The holding time may be changed by an authorized service technician only.



Changing the drying time

The duration of the drying time can be increased or decreased according to the characteristics of the load. When changing the drying time, ensure that the load is always dry at the end of a sterilization cycle in order to avoid wicking of moisture and, potentially, microorganisms from hands, gloves or environmental surfaces.

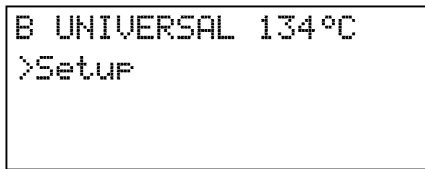


After selecting a cycle, press UP or DOWN until the SETUP option appears and confirm (OK). Scroll the sub-menu options by pressing UP or DOWN (the current value is displayed) and follow the instructions in the table below.

| MENU | SUB-MENU | WHAT IT DOES AND HOW TO SET IT | |
|-----------------|--|--------------------------------|--|
| Setup | Set as default (*) | Yes | Sets the cycle as the default cycle, means it will appear first on the start screen. After pressing OK, press OK on YES to set the cycle as the default cycle (the other cycles will be automatically set to NO); press BACK to exit without saving. |
| | Hide (*) | Yes | Unhides/hides a cycle. Once a cycle is hidden, it will no longer be visible in the menus and thus it will be impossible to launch it. |
| | | No | After pressing OK you can scroll between YES and NO with the UP and DOWN buttons. Press OK on YES to hide the cycle, press OK on NO to unhide it, press BACK to exit without change. |
| Drying time (*) | Sets the duration of the drying phase. | | After pressing OK, an asterisk will appear near the current value, indicating that it can be changed by pressing UP or DOWN. After programming the desired value, press OK to confirm or BACK to exit without saving. |

Cycle in progress

Information displayed on the screen while a cycle is in progress

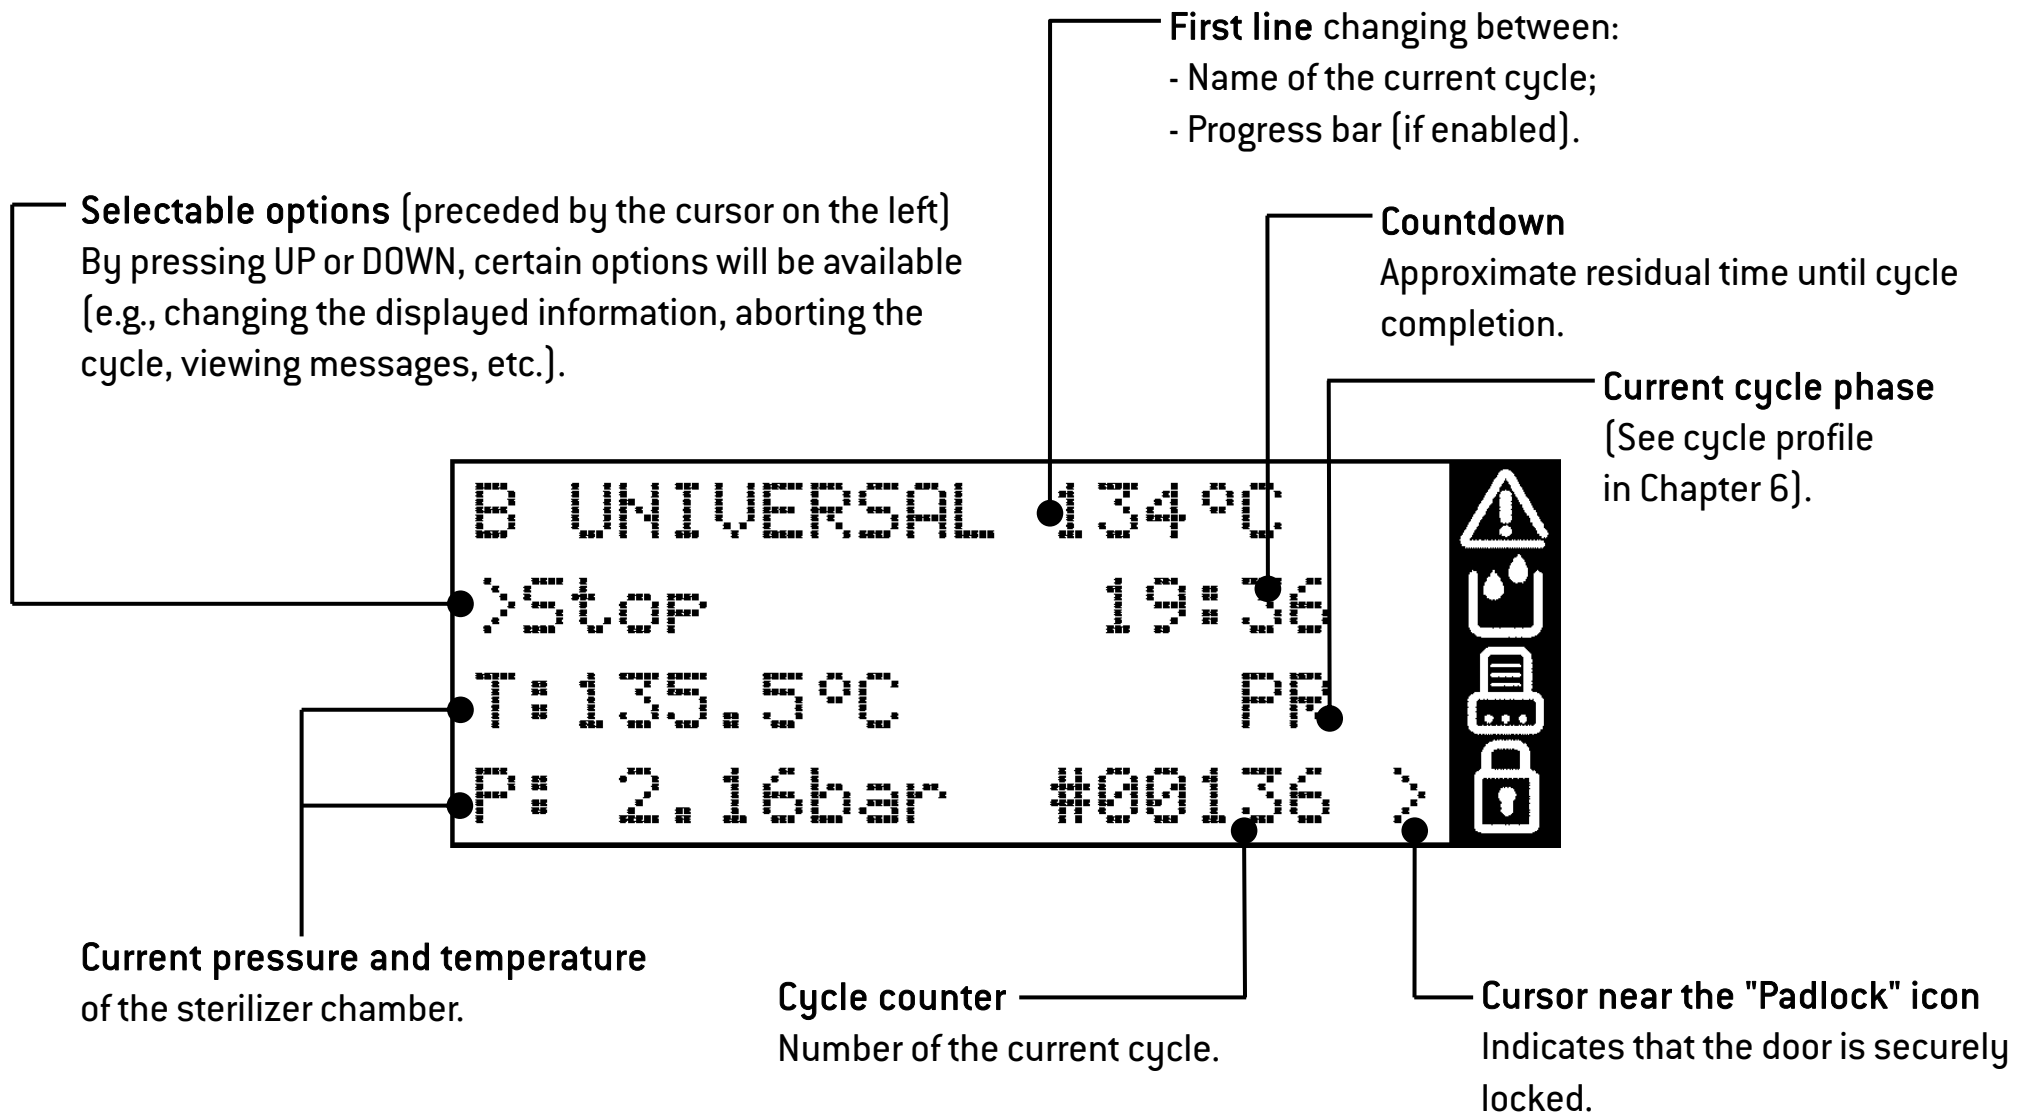

Cycle in progress


INFO screen and menu options

While a cycle is in progress, you can view the main cycle parameters in real time.

On the “cycle in progress” screen, press UP or DOWN until the INFO option appears. Other menu items are also available at this stage.

```


B UNIVERSAL 134°C
>Info
T:135.5°C      PR
P: 2.16bar    #00136 >
    
```



Then confirm with OK.

```

          Info
Cycle      10:13
Phase      0:13
The low    135.5°C >
    
```



The current parameters of the cycle in progress are displayed.

Press UP or DOWN to view the complete list of values (see table below).

Press BACK to return to the standard “cycle in progress” screen.



| Screen title | Info |
|---------------------------------------|------------------|
| Cycle time | Cycle 0:00 |
| Phase time | Phase 0:00 |
| Lower heating element temperature | The low 40.25°C |
| Upper heating element temperature | The up 40.25°C |
| Steam pressure | P1 0.65bar |
| Temperature in the chamber | Tst 40.25°C |
| Lower heating element power output | Pwr-he low 865W |
| Upper heating element power output | Pwr-he up 865W |
| Theoretical temperature | Tth1 40.25°C |
| Additional chamber sensor temperature | T6-EPIN 40.25°C |
| Mains voltage | U. mains 229.12V |
| Mains frequency | F. mains 50Hz |
| Total water injected | H2O 57cc |
| Water conductivity | H2O 9.2uS |

Legend of the parameters displayed when scrolling the INFO screen.


Manual stop

While a cycle is in progress, you can abort it manually at any time.



Press UP or DOWN until the STOP option appears preceded by the cursor, then proceed as shown below:

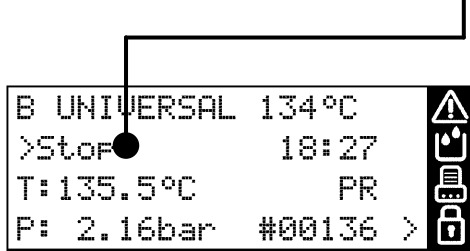

Confirm STOP (OK)

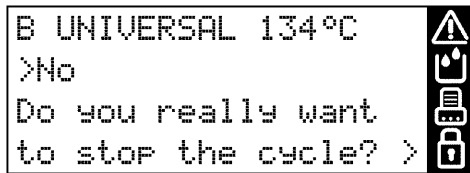


Press DOWN until YES appears.

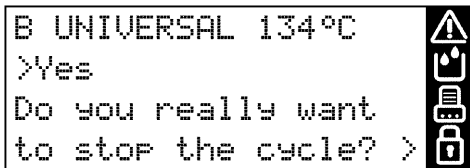

Confirm (OK) YES



Before the cycle abortion is confirmed, the abortion procedure can be interrupted at any time; press BACK several times until you get to the “cycle in progress” screen and the cycle will go on as originally programmed.

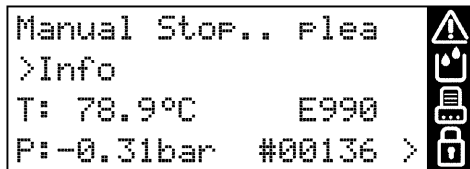


Once a cycle is aborted, a reset phase commences to safely release any steam pressure from the chamber. This may take several minutes. Do not switch off the sterilizer! Wait until the reset phase is completed.

At this stage you can access some menu items by pressing UP or DOWN.

When selecting the INFO option (see picture) you can view the sterilizer parameters in real time (see previous page).

Manual stop

B UNIVERSAL 134°C
Manual stop E990
Press "back icon" >

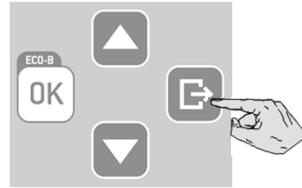


When the reset phase is over, press BACK

One of the following messages appears:

B UNIVERSAL 134°C
>Unlock door
Manual stop E990
Load not sterile ●>
Ster.cond.achieved
dryin9 interrupted

The message LOAD NOT STERILE means that the load is not sterile. Do not use items on patients!


The message DRYING INTERRUPTED means that the load might be wet. Wet items are for immediate use only!



Press OK to unlock the door as requested in the second line of the screen.

(a waiting message appears while the door is unlocking)

B UNIVERSAL 134°C
Open door!




Open the chamber door and remove the load, or repeat the sterilization cycle.

End of a sterilization cycle


```
B UNIVERSAL 134°C
>Unlock door

Cycle completed >
```



```
B UNIVERSAL 134°C

Open door!
```



```
B UNIVERSAL 134°C
>Unlock door
End of alarm E331
Load not sterile >
```



When a cycle is successfully finished, the **CYCLE COMPLETED** message appears on the screen and the “Unlock door” option is preceded by the cursor.

At this stage you can press **DOWN** or **UP** until the **INFO** option appears; confirm **INFO** to view the cycle parameters (see previous pages).

This is only possible prior to unlocking the chamber door.

Confirm **[OK]** to unlock the door (the cursor near the “padlock” icon disappears).

Wait the door to unlock, then open the chamber door.

If an alarm message appears at the end of the cycle, consult Chapter 8 (Troubleshooting) and, if the problem persists, call for technical service.


Remove the load from the chamber.



WARNING! THE LOAD AND THE STERILIZER ARE HOT!

Use the tray holder (or cassette holder) to remove the load!

Do not touch the chamber, the inner porthole and the internal fittings as long as they are hot.

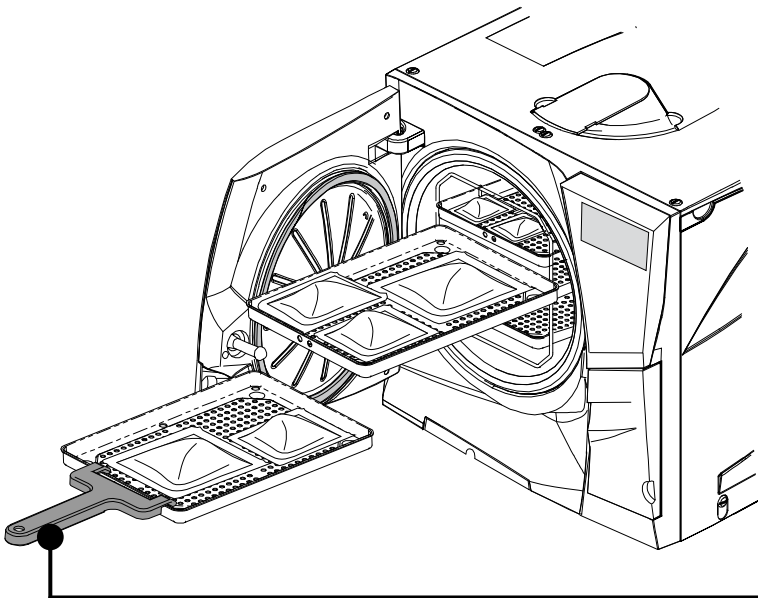

7. Maintenance



Before carrying out any maintenance on the sterilizer, switch the unit OFF and remove the mains cable.



Before accessing the chamber and the connected parts, be sure that the sterilizer is cold.



Follow the instructions in this chapter when carrying out any maintenance on the sterilizer.

Maintenance program


The maintenance program is outlined in the table on the next page.

It includes the replacement of certain wearing parts (consumables) which is imperative to ensure the safe and faultless operation of the sterilizer.

Maintenance counters

The sterilizer keeps track of the age of consumables by keeping memory of the number of cycles executed since the last replacement.

When one counter reaches the maximum, a replacement message appears on the screen and the consumable needs to be replaced; replace the consumable.

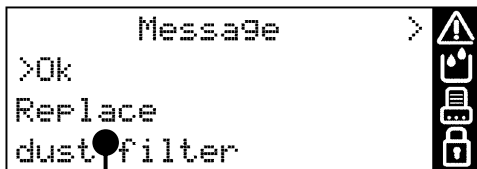


Maintenance program

| MAINTENANCE PROGRAM TABLE | | | | | | | | |
|---------------------------|-----------------|---|-------------|--------------|-------------|------|-------------|------|
| Frequency (*) | # of cycles (*) | Operation | Consumable | Performed by | | | | |
| Monthly | 50 | Clean the door seal and the chamber face side | See ANNEX 9 | User | | | | |
| | | Clean the chamber, trays and the rack | | | | | | |
| | | Clean the chamber filter | | | | | | |
| | | Clean the external sterilizer surfaces | | | | | | |
| | | Clean the steam diffuser plate | | | | | | |
| 3 months | 400 | Replace the bacteriological filter | | | See ANNEX 9 | User | | |
| | | Replace the dust filter | | | | | | |
| 6 months | 800 | Clean both water tanks | | | | | See ANNEX 9 | User |
| Yearly | 800 | Replace the door seal | | | | | | |
| 5 years | 4000 | General check and service | | | | | | |

(*) whichever occurs first

Monthly or 50-cycle maintenance

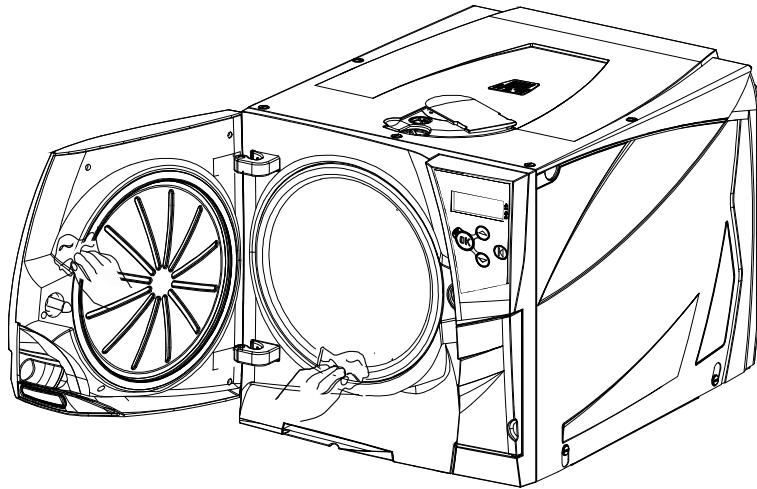

Cleaning the door seal and the chamber face side


Clean the door seal and the outer edge of the chamber with a non-abrasive cloth moistened with water. If you use a detergent solution, be careful not to get in contact with the plastic body of the front cover.

Rinse with clean water.

Do not use abrasive products, cutting tools or sharp objects.

Cleaning the chamber and the chamber accessories

Remove the trays, the chamber rack and the steam diffuser plate (see section “Chamber Furniture” in Chapter 4)

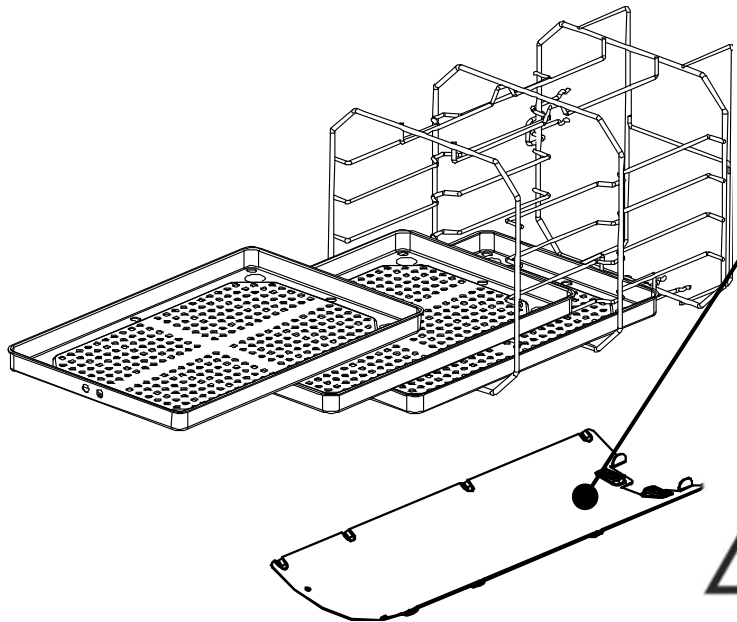

Clean the chamber with a damp sponge and a mild detergent solution paying attention not to bend or damage the temperature probe inside the sterilizer chamber. Rinse with water.

Clean the steam diffuser plate, the trays and the tray rack with a damp sponge and a mild detergent solution. Rinse with water.


Reposition all pieces of the chamber accessories properly.

Ensure that the steam diffuser plate is correctly placed and engaged, as this is essential for the sterilization process.



The trays, the tray holder and the steam diffuser plate may also be cleaned in a washer disinfectant.

Monthly or 50-cycle maintenance

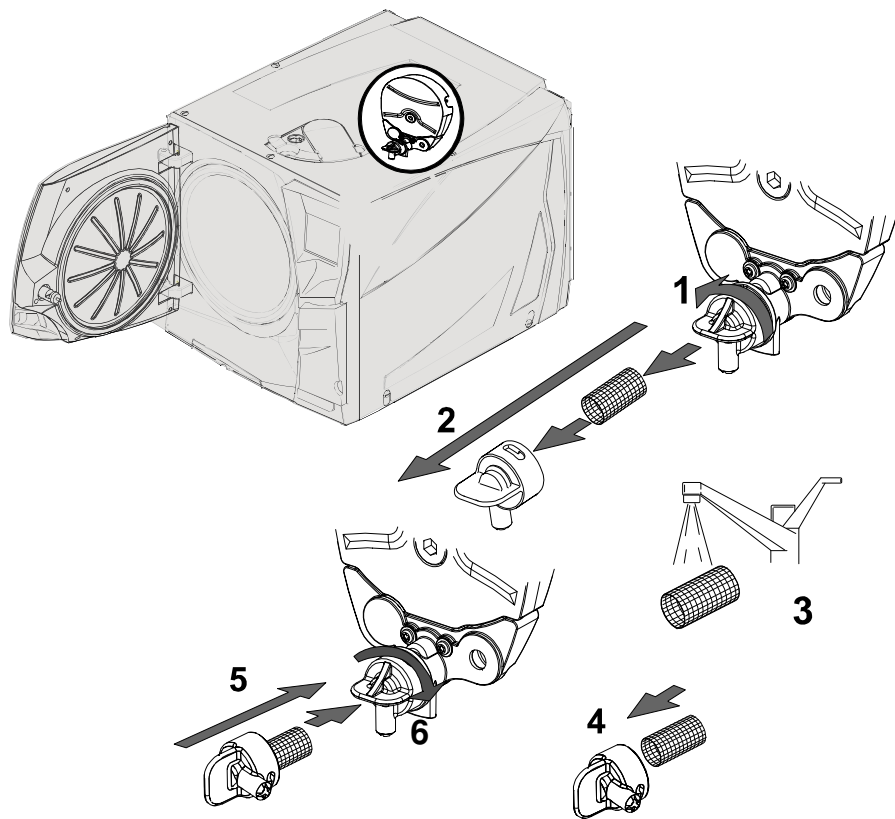

Cleaning the chamber filter

Empty the sterilizer chamber by removing the trays and the rack.

1–2: Remove the filter cap at the back of the chamber (bottom/center) by turning it counter-clockwise.

3: Remove the cartridge filter and rinse it with tap water.

4–5–6: Insert the filter in the cap, attach the filter cap and lock it by turning clockwise.

Cleaning the external surfaces of the sterilizer

Clean all external sterilizer covers with a slightly damp cloth moistened with water.


For better cleaning results, clean with W&H MC-1000 cleaning solution.

NOTICE: Never use any other disinfectant, detergent or abrasive product, as they might result aggressive for the external covers and damage them.



NOTICE: Never use any other disinfectant, detergent or abrasive product, as they might result aggressive for the external covers and damage them.

3 month or 400-cycle maintenance

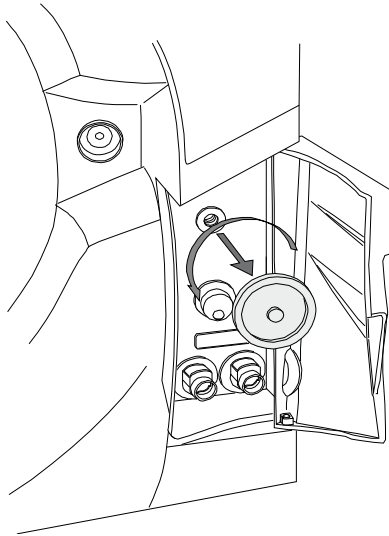

Replacing the bacteriological filter


Open the service door.

Unscrew the bacteriological filter by hand (counter-clockwise).

Screw on the new bacteriological filter (clockwise) and tighten it snug.



Remember to reset the counter after replacement (see following pages).

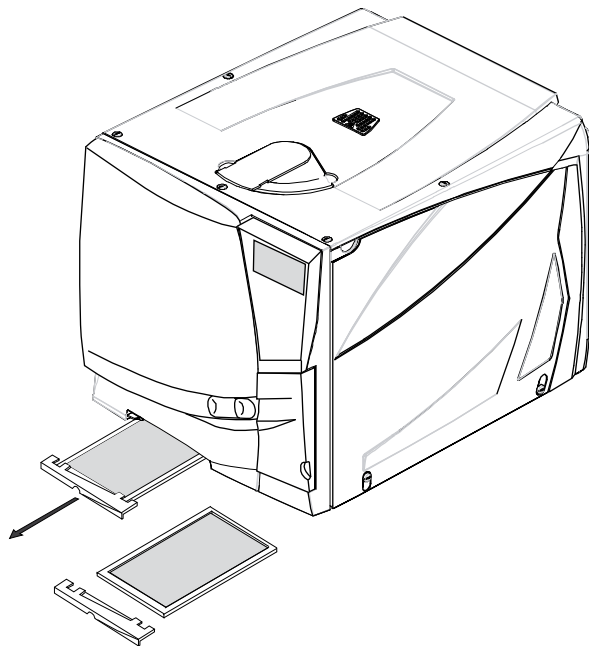

Replacing the dust filter

Pull out the dust filter from underneath the sterilizer.

Detach the used filter from the handle.



Attach the new filter to the handle.

Slide the filter back into its original position.



Remember to reset the counter after replacement (see following pages).

6 month or 800-cycle maintenance

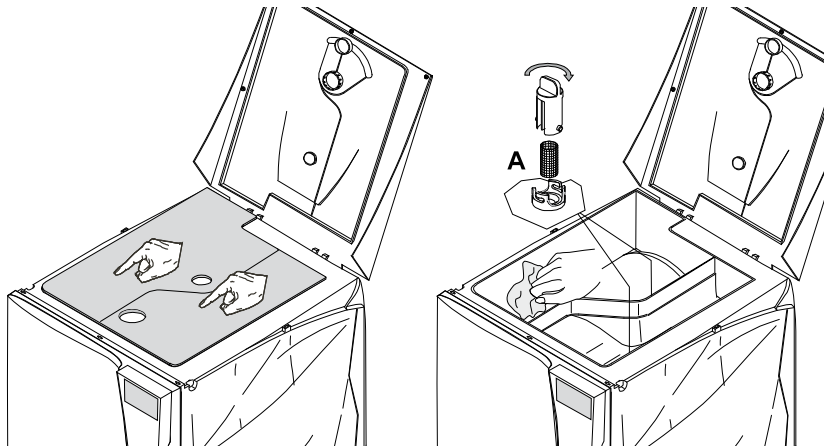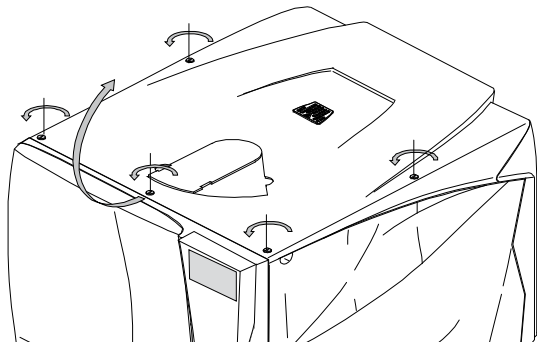

Cleaning the water tanks

Switch OFF the sterilizer and disconnect the mains cable.

Completely drain both tanks.

Leave the drain tube attached to one of the drain quick connectors.

Turn the 5 screws of the tank cover a $\frac{1}{4}$ with the use of a screwdriver (a coin works as well) and lift the cover to gain access to the tanks. Tap with your fingers on the rubber membrane to remove any condensate.

Remove the rubber membrane; clean and dry it.

Clean the internal tank surfaces with a soft sponge moistened with water. For better cleaning results, clean with W&H MC-1000 cleaning solution. Use a small non-abrasive brush to clean the areas that are difficult to reach.

Rinse the tank thoroughly, until all residuals of dirt and detergent have been eliminated. Make sure the drain tube is connected to the tank you are cleaning (left tank – grey colored connector; right tank – blue colored connector) to drain the detergent solution.

Only when both tanks are clean, remove the internal filters (A), clean them with tap water and put them back into their position. Reposition the rubber membrane.

Close the cover and tighten the 5 tank cover $\frac{1}{4}$ turn screws .

Disconnect the drain tube.





Never use any other disinfectant, detergent or abrasive product, as they might result aggressive for the tank material.



When cleaning the tanks, be careful not to touch the water level sensors. If misplaced or misaligned from their original position, the operation of the sterilizer could be impaired.

1 year or 800-cycle maintenance

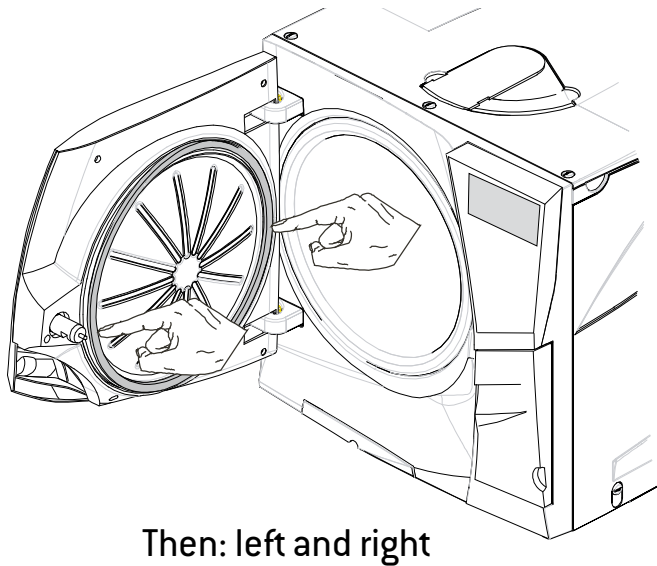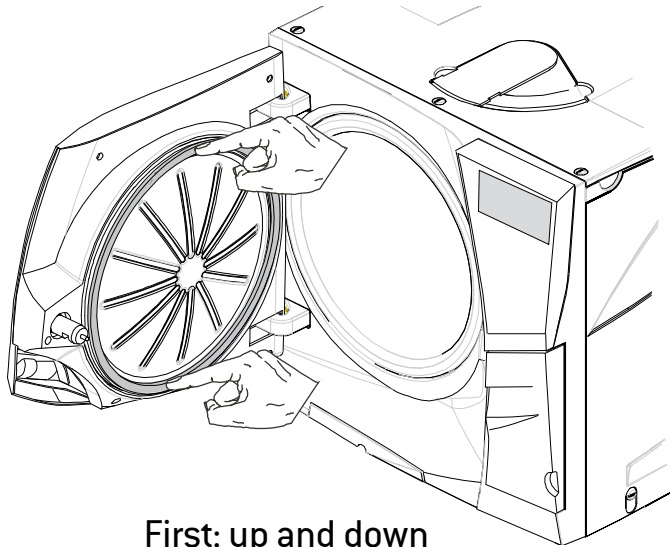

Replacing the door seal

Fully open the chamber door.

Pull out the used door seal by hand (easy if seal and fingers are dry).

Carefully clean the seal seat and the chamber face side with a cotton swab.

Moisten the new seal with water. This will make placement much easier!

Insert the new seal in the sequence as illustrated in the pictures to the left.

Complete the operation by evenly inserting the seal on the entire circumference; ensure the seal does not stick out (no bumps or deformations)!



Before using the sterilizer, wipe any residual water and check for perfect tightness of the seal by running a Vacuum test and a Helix test.



Remember to reset the counter after replacement (see following pages).

4000 cycle/5 years general check and service



Regular service is imperative to ensure continuous and effective operation of the sterilizer.


It is recommended to carry out a general service every 4000 cycles or five years by an authorized service technician.




The service includes replacement of consumables and other important internal components, a check of the entire unit with special care for the safety systems, and cleaning of areas and components that cannot be accessed by the user.

| REPLACEMENT PARTS | CLEANING | CHECKS |
|---|---|--------------------------------------|
| Solenoid valves Vacuum pump internal parts | Sterilization chamber and external surfaces | Pneumatic connections |
| | Chamber filter | Electrical connections |
| | Internal cleaning, with particular care for the condenser fins and the main board | Temperature and pressure calibration |
| | | Door locking system |
| | | Pressure safety valve |
| Steam diffuser plate | Safety systems | |


Resetting the maintenance counters

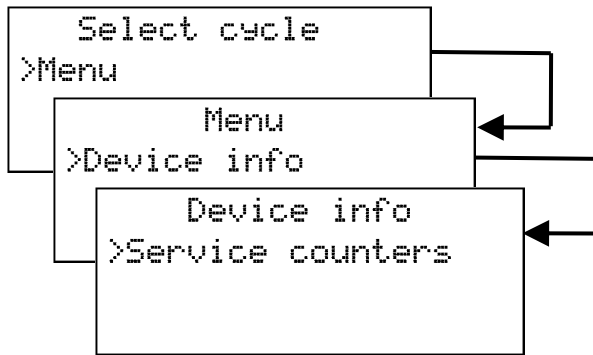

Use the UP, DOWN and OK buttons to browse the menu, choosing the following options in sequence: MENU – DEVICE INFO – SERVICE COUNTERS.

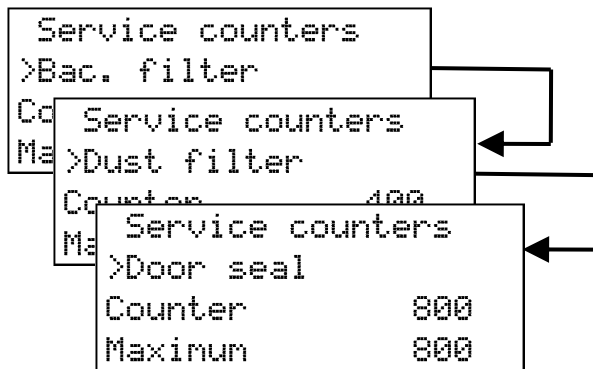

Scroll to the concerned consumable by pressing UP or DOWN. The consumable status (number of cycles executed and maximum lifespan of the consumable) is displayed in the third and fourth line of the display. Press OK to select the concerned consumable.

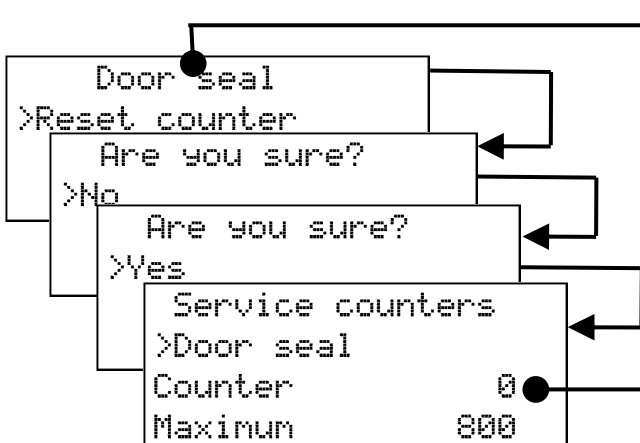


After selecting, the concerned consumable appears in the first line.

The RESET COUNTER option is displayed: confirm it with OK.


A confirmation request appears: scroll the answer to YES by pressing UP or DOWN and then confirm with OK.

After being reset, the consumable counter shows zero.


8. Troubleshooting, alarms and messages

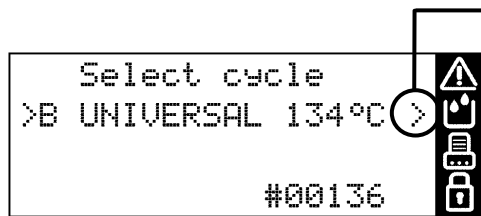

If the cursor appears to the left of one or more icons, there is related information pending.
All messages can be viewed by means of the MESSAGES sub-menu.

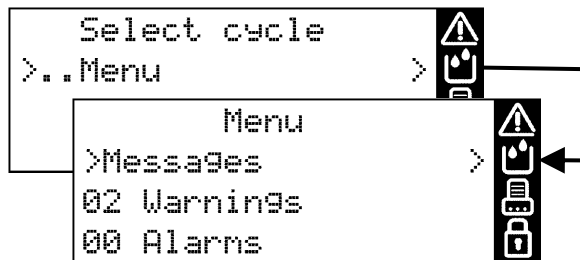

Use the UP, DOWN and OK buttons to browse the menu, choosing the following options in sequence: MENU - MESSAGES

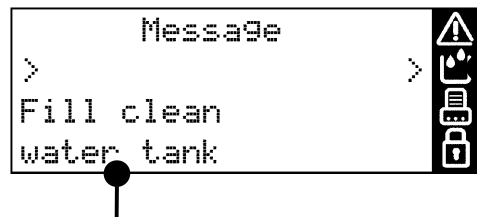

If there is more than one message pending, you can scroll within messages with UP or DOWN.

The icon that is preceded by the cursor is related to the pending message.







The cursor that precedes the icon disappears as soon as the relevant message has been read and the condition that gave rise to the message has been fixed.



The cursors that precede the message icons are not visible while a cycle is in progress.

Messages

| ICON | MESSAGE | DESCRIPTION/ACTION REQUIRED |
|--|--|--|
|  | - | The chamber door is locked; no action required. |
|  | Fill clean water tank | The water level inside the clean water tank is below the minimum. Fill the clean water tank. |
| | Drain used water tank | The water level inside the used water tank is at maximum level. Drain used water tank. |
| | Bad water quality Check H2O supply | Check the external sterilizer water supply. You might have to replace filter cartridges – drain clean water tank and follow instructions for use of water filtration system. |
| | Non conform water Do not use the sterilizer!! | The distilled/demineralized water in the clean water tank is of poor quality. Drain the tank and refill it with water of good quality; refer to ANNEX 7 |
| | Bad water quality STOP using the sterilizer!! | |
|  | WARNING Chamber is hot!! | Don't touch the chamber or the load with bare hands: high temperature, risk of burns! |
| | Replace bac. filter | The bacteriological filter needs to be replaced. |
| | Replace dust filter | The dust filter needs to be replaced. |
| | Replace door seal | The door seal needs to be replaced. |
| | 4000 cycle service recommended | The 4000 cycle overhaul needs to be performed. Call for service. |
| | WARNING ! Low battery | The CPU board battery needs to be replaced. Call for service. |
| |  | PC connection lost Check cables/PC |
| Printer not ready | | Cycle report printer configured but not detected (disconnected or not powered). |
| Label printer not ready | | Label printer configured but not detected (disconnected or not powered). |
| File save error | | File saving error (check presence and connection of the USB drive). |
| USB4 error See user manual or contact service for details | | Error in the USB communication (between the main board and the USB4 board) |
| HTML save error - See user manual | | Error in savng the HTML cycle report |
| SCL save error - See user manual | | Error in savng the SCL cycle report |
| Check Usb device - See user manual | | Bad USB device |



NOTE: for any message not listed in this table, call service.

Alarm stop

In case certain important sterilization parameters are not met, the sterilizer will generate an alarm code and abort the cycle automatically.


The sterilizer enters into a reset phase; a wait message and an alarm code are displayed on the screen.

```
ALARM.. Please wai
>Info
T: 78.9°C      E331
P: +0.31bar   #00136 >
```

At this stage select and confirm "Info" to view the sterilizer parameters (see Chapter 6 of this manual).

Do not switch off the sterilizer: It will take some time (several minutes) to reset the system and reach safe conditions in the sterilizer chamber before it is possible to open the sterilizer door and remove the load.


```
B UNIVERSAL 134°C
End of alarm E331
Press "back icon" >
```

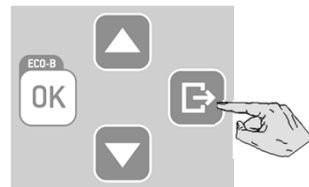

Alarm end

When the reset phase is over, you will be asked to press BACK to get to the "Unlock door" option.

```
B UNIVERSAL 134°C
>Unlock door
End of alarm E331
Load not sterile >
Ster.cond.achieved
drying interrupted
```




Confirm (OK) to unlock the door.

While the door is unlocking, a waiting message is displayed.

The message **LOAD NOT STERILE** means that the load is not sterile. Do not use items on patients!

The message **DRYING INTERRUPTED** means that the load might be wet. Wet items are for immediate use only!

```
B UNIVERSAL 134°C
Open door!
```



Open the chamber door and remove the load.



Water could be present in the chamber when opening the door: prevent spilling (e.g., place a towel under the chamber door).

Alarms

| Alarm code | DESCRIPTION | ACTION |
|------------|--|---|
| E010 | Power failure during a cycle | Load cannot be considered sterile. Repeat the cycle. |
| E02x | Internal voltage error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E041 | Cycle counter lost | Switch the sterilizer OFF and ON. If the problem persists call service. NOTE: Initiating a sterilization cycle is still possible. |
| E042 | Internal clock error | Set date and time - Switch the sterilizer OFF and ON. If the problem persists call service. NOTE: Initiating a sterilization cycle is still possible. |
| E060 | Internal voltage error | Disconnect optional accessories from 24VDC rear plug - switch the sterilizer OFF and ON. If the problem persists call service. |
| E080 | Internal overheating | Check the dust filter and ensure that the sterilizer fan is not blocked. |
| E090 | Internal voltage error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E100 | Phase timeout | Check water level in the clean water tank. Reset the thermal overload. If the problem persists call service. |
| E101 | Internal probe error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E102 | Phase timeout | Check water level in the clean water tank. Reset the thermal overload. If the problem persists call service. |
| E107 | Overpressure during the pre-vacuum phase | If the problem persists call service. |
| E121 | Internal probe error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E130 | Overpressure during the sterilization phase | Clean the chamber and the chamber furniture from residuals of detergents, disinfectants and other chemicals. Replace the clean water if it is suspected to be contaminated with chemicals. Ensure all the load is clean rinsed and free from any chemicals before sterilizing. Repeat the cycle. If the problem persists call service. |
| E131 | Temperature fluctuation during the steril. phase | |
| E140 | Low pressure during the sterilization phase | |
| E150 | Low temperature during the sterilization phase | |
| E160 | Over temperature during the sterilization phase | |
| E163 | Overpressure detected | |
| E180-E181 | Internal probe error. | Switch the sterilizer OFF and ON. If the problem persists call service. |



NOTE: for any alarm not listed in this table, call technical service.



Alarms

| Alarm code | DESCRIPTION | ACTION |
|--------------------------|--|--|
| E182 | Pressure drop timeout | After the process phase the pressure took too long to drop to the atmospheric pressure. If the problem persists call service. |
| E184 | Overtemperature detected | If the problem persists call service. |
| E215 | Fan blocked or faulty electronic control | Call service. |
| E230 | Internal probe error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E231 | Overtemperature detected | If the problem persists call service. |
| E232-E233-E234 | Internal probe error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E240-E243 | Lower heating element error | Wait for the chamber to cool down. Reset the thermal overload (see next page). If the problem persists call service. |
| E250-E251 | Upper heating element error | If the problem persists call service. |
| E310-E320-E33x-E380-E390 | Vacuum timeout | Check the door seal; clean or replace if necessary. Clean the chamber face side. Clean the chamber filter. If the problem persists call service. |
| E510 | Door motor: failure after cycle completion | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E520 | Door motor: locking timeout | If the problem persists call service. |
| E570 | Door motor: unable to detect the door position | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E580 | Door motor: door locked check signal lost | If the problem persists call service. |
| E59x | Door motor error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E950 | Internal memory error | Switch the sterilizer OFF and ON. If the problem persists call service. NOTE: Initiating a sterilization cycle is still possible. |
| E95x-E96x | Internal memory error | Switch the sterilizer OFF and ON. If the problem persists call service. |
| E990 | Manual stop | The cycle has been aborted by the user. Re-process the load. |



NOTE: for any alarm not listed in this table, call technical service.

Resetting the thermal overload

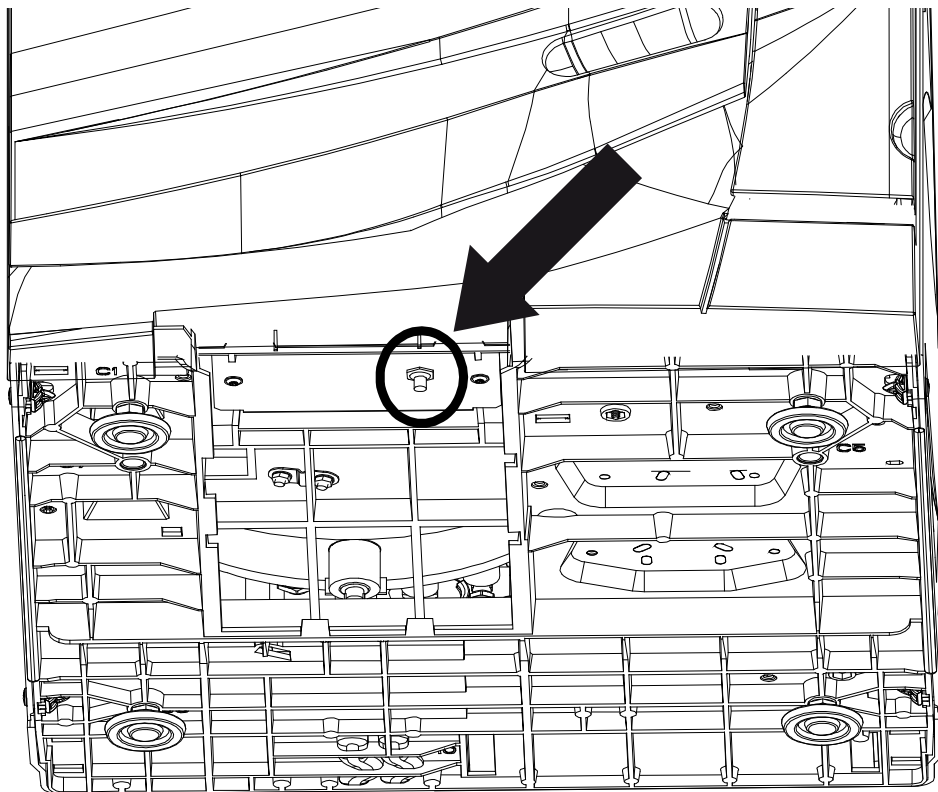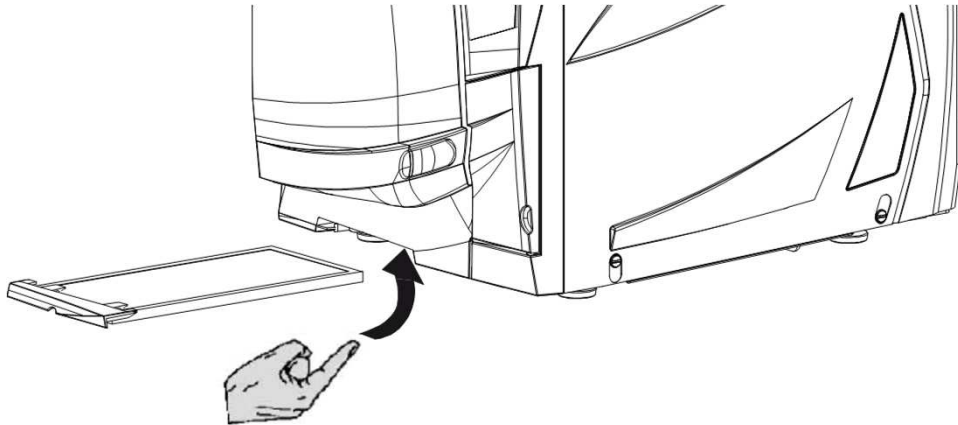

A safety thermostat is fitted on the sterilizer to prevent overheating of the electric heater.

If the safety thermostat operates because of too high temperatures, the alarm E240 or a timeout alarm is generated.

If this happens, proceed as follows:

- Switch the sterilizer OFF and remove the mains cable.
- Wait for the sterilizer to cool down.
- Remove the dust filter.
- Slide your hand underneath the sterilizer where the dust filter was located and push on the reset button of the thermostat switch (see pictures to the left).
- A click sound will indicate that the thermostat switch has been reset.
- Insert the dust filter back into its original position.
- Connect the mains cable and switch the sterilizer ON.
- Wait for the sterilizer to finish the alarm reset phase and follow the instructions on the display.

If the thermostat operates repeatedly, call technical service.

Troubleshooting

| PROBLEM | POSSIBLE CAUSE | SOLUTIONS |
|---|---|---|
| The sterilizer remains switched OFF. | The main switch or network circuit breaker is OFF | Activate the main switch or network circuit breaker (ON). |
| | No voltage at the socket | Check the electric circuit. |
| | The mains cable is not properly connected | Attach the cord set properly. |
| Water is leaking at the front of the sterilizer | Leaks through the chamber door seal | Clean or replace the door seal. Clean the chamber face side. |
| | Internal leak. | Call technical service. |
| The cycle commences but there is no pressure/temperature rise | The thermal overload switch is open | Reset the thermal overload switch (see “Resetting the thermal overload” in this manual). |
| | Electric – electronic fault | Call technical service. |
| At the end of the cycle, there is residual water in the chamber | Sterilizer not properly levelled | Properly level the surface the sterilizer is placed on. |
| | Overloaded chamber | Comply with the maximum load weight limits for each type of load. Always use the chamber rack for trays and cassettes. |
| | Chamber filter clogged | Remove and clean the chamber filter. |
| | Load incorrectly placed | Follow the recommendations as listed in ANNEX 2. |
| Corrosion or spots on instruments | Tap water on instruments when placed in the sterilizer | Ensure that instruments are dry before they are placed in the sterilizer. |
| | Use of water of poor quality or water containing chemical substances | Drain both water tanks. Use water of good quality (see ANNEX 7). |
| | Organic or chemical residues on the instruments | Clean, rinse and dry instruments before placing them in the sterilizer (see ANNEX 2). |
| | Contact between instruments of different materials | Ensure that instruments of different materials do not touch (aluminum, carbon or stainless steel, etc.); place them on different trays or cassettes or pouch them (refer to ANNEX 2). |
| | Scale deposits on the chamber | Clean the chamber and use water of good quality (refer to ANNEX 7). |
| Instruments are turning brown or black. | Incorrect temperature selected | Select a sterilization cycle featuring a lower sterilization temperature. Follow the instructions of the instrument manufacturer. |
| The cycle report printer does not work | Printer not properly connected or not powered | Check the data and the power connection to the printer. |
| | Serial port not configured | If the printer is connected directly: configure the serial port to “Printer” (see Table 2). If connected via PC/Logger: configure the serial port to “PC/Logger” (see Table 2). |
| | The cycle is in progress and the automatic report printing is enabled | You are trying to print a stored cycle but the printer is busy to print the data of the cycle in progress: the requested printout will be queued. NOTE: The max. queue is 5 cycles. Longer queues will be ignored. |
| No cycles are stored in the cycle history menu | Power board replaced by service | These service steps cause loss of memory. |
| | Serial number re-entered by service | |

Troubleshooting

| PROBLEM | POSSIBLE CAUSE | SOLUTIONS |
|--|---|--|
| When starting a cycle, the chamber door locks but re-opens immediately. The “Open the door” message appears. | Door seal not properly placed; seal sticking out | Ensure that the door seal is evenly inserted on the entire circumference. |
| | OK button was pressed twice to launch the cycle | Try again by pressing OK only once. |
| | Door jammed by external objects or by the load itself | Remove any objects interfering with the chamber door. Check the door does not force against the load or the chamber furniture. |
| When the sterilizer is connected to an automated water supply system: There is no clean water in the tank, but the automatic water filling does not start. | Water fill system (optional) not installed | Install a water fill system. |
| | Water fill system (optional) not connected | Connect the water fill system to the sterilizer (see ANNEX 7 for water quality requirements). |
| | Water fill system (optional) not configured | Enable the water fill system in the “Configuration” sub-menu (see Chapter 5, Table 2). |
| | When the water fill system attempted to fill the tank, water was temporarily unavailable | Since water tank filling is attempted only once in-between cycle execution, this event inhibits water feeding. Switch the sterilizer OFF and then ON again. Check the external water supply system. Check for water leaks from the sterilizer. |
| The sterilizer enters into “Sleep mode” immediately after opening the chamber door. | The chamber door has not been opened after the previous cycle had finished and the “Sleep mode delay” has expired | Press any button on the control panel to exit from “Sleep mode”. |
| At the end of the cycle the display reads “Open the door” but opening the door is impossible. | The chamber is in vacuum due to an internal malfunction | Switch the sterilizer OFF: this will release any internal pressures allowing the chamber door to be opened. Call technical service if the problem persists. |
| | The bacteriological filter is blocked | Remove the bacteriological filter to get the pressure released. Replace the filter. Note that bacteriological filters need to be replaced every 400 cycles. |
| The sterilization (PROCESS) phase of a sterilization cycle was longer than expected. | The chamber temperature dropped below the minimum threshold and the software performed a successful recovery | Wait for cycle completion. If the problem occurs frequently, call technical service. |



Before sending the sterilizer for technical service, remove the mains cable, empty both water tanks and use the original or appropriate packaging.

9. Recycling and disposal



LINA sterilizers are mainly built from fiber-reinforced polymers, metals and electronic components.

In case of disposal:

- separate the various components according to the materials they are made of;
- drop the sterilizer with a company that specializes on the recycling of related products;
- do not abandon the sterilizer in unsecured places;
- always refer to current/applicable laws and rules in the country of use.


The same instructions apply to disposal of all used consumable parts.


ANNEX 1. Technical data

| TECHNICAL DATA | |
|---|---|
| Usage environment | Indoor |
| Electrical supply: | 200 - 240 V AC – 50/60 Hz, single - phase |
| Nominal voltage: | 200 - 240 V AC ±10% |
| Max. current: | 10 A |
| Sterilizer: | |
| Working temperature: | from +5°C to +40°C |
| Working relative humidity: | Max. RH 80% up to 31°C, linearly decreasing to 50% at 40°C |
| Storage temperature /rel. humidity: | / -20°C to +60°C/0-90% (with empty tanks) |
| Max altitude: | 3000m asl |
| Min. atmospheric pressure: | 0.6 barA |
| Overall dimensions: | W: 45 cm/H: 44 cm/D: 60cm |
| Min. space required (feet in forward position) | W: 47 cm/H: 49 cm/D: 53 cm |
| Min. space required (feet in rearward position) | W: 47 cm/H: 49 cm/D: 46 cm |
| Size of the door movement: | W: 36 cm/H: 38 cm/D: 34 cm |
| Weight empty: | 39 kg (LINA 17), 40 kg (LINA 22) |
| Max. weight (fully loaded): | 50.5 kg (LINA 17), 52.5 kg (LINA 22) |
| Weigh per support area | 30.9 kN/m ² |
| Max. heat output: | 3000 KJoule/hour |
| Pressure safety valve: | 2.6 bar |
| Safety thermostats | 330°C (lower chamber) – 180°C (upper chamber) |
| Sterilizer chamber: | |
| Total volume: | Ø: 250 mm/D: 362 mm (LINA 17) Ø: 250 mm/D: 440 mm (LINA 22) |
| Usable space (for all cycles) | W: 195 mm /H: 195 mm/D: 297 mm (LINA 17) W: 195 mm /H: 195 mm/D: 390 mm (LINA 22) |
| Bacteriological filter: | 0.3 µm |
| Distilled or demineralized water: | |
| Water quality: | Fulfilling EN 13060 Ann. C (conductivity < 15µS/cm) |
| Average water consumption: | 0.40 to 0.75 litres/cycle |
| Tank volume: | Clean water 4 l – Used water 3.5 l |
| External water supply: | To be compliant with IEC61770 |
| Pressure: | min. 2 bar – max. 8.6 bar |
| Flow: | min. 0.25 – max 0.5 l/min |
| Max. temperature: | 35 °C |
| Communication with other devices: | 1 serial port - (optional: 1 USB port + 1 additional serial port) |
| Other | Fully micro-processor controlled, process evaluation system according to EN13060. Programmable sleep-mode. |


| CONFORMITY | |
|---|--|
| STERILIZER complying with the following Regulations, Directives and Standards: | |
| 93/42/EEC | Medical Device Directive (MDD) |
| PED 2014/68/EU | Pressure Equipment Directive (PED) |
| 2012/19/EU | Waste Electrical and Electronic Equipment (WEEE) |
| EN 13060 | Small steam sterilizers |
| IEC 61010-1 | Safety requirements for electrical equipment for measurement, control and laboratory use, general requirements |
| IEC 61010-2-040 | Safety requirements for electrical equipment for measurement, control and laboratory use; particular requirements for sterilizers and washer-disinfectors used to treat medical materials. |
| EN 61326-1 | Electrical equipment for measurement, control and laboratory use: EMC requirements; general requirements. |

LINA sterilizers can be validated in accordance to EN ISO 17665-1.

| RECOMMENDATIONS FOR VALIDATION |
|---|
|  |



LINA 17

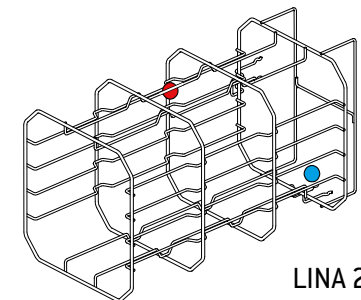

LINA 22

For further details please refer to the Qualification / Validation guide for sterilization cycles of W&H sterilizers.

ANNEX 2. Maintenance of dental handpieces

External disinfection

This procedure reduces the risk of infection during cleaning and maintenance of the instrument.

Wear protective gloves during disinfection.

Refer to the instructions of the instrument manufacturer.

Avoid using abrasive disinfectants (pH-value 2.5 – 9; no chlorine based disinfectants).

We recommend the use of disinfectant wipes rather than spray disinfection.

Do not immerse instruments in disinfectants.

Residual disinfectants on instruments can cause extensive damage to your instrumentation during sterilization (oxidation, alteration of technical characteristics of seals, rubbers, fiber optics, etc.).

External cleaning

This procedure involves the removal of residues (blood, dentine, etc.) that adhere to critical areas such as spray outlets, light ports, knurling etc.

Wear protective gloves during cleaning.

Refer to the instructions of the instrument manufacturer.

Use a soft, damp brush and take care not to scratch the surface of the light ports.

Lubrication

Once the instrument has been disinfected, cleaned and dried (free from residues), it must be lubricated **prior to** sterilization.

Follow manufacturer's instructions for proper lubrication.

Packaging

In order to preserve sterility, rotating instruments should be wrapped/bagged prior to sterilization. Follow the manufacturer's packing instructions when using sterilization packaging (also see "Sterilization load preparation" in ANNEX 3 of this manual).

ANNEX 3. Sterilization load preparation

Cleaning the instruments

Clean all instruments thoroughly prior to sterilization.

If possible, clean instruments immediately after use; always follow the instrument manufacturer's instructions.

Remove all traces of disinfectants and detergents.

Rinse and dry carefully all instruments.

Lubricate dental handpieces after cleaning and prior to sterilization in accordance with the manufacturer's instructions.



The instruments must be carefully rinsed and dried prior to sterilization.

Any residual of chemicals (like cleaning and disinfection products), could affect the purity of the steam and consequently the whole sterilization process, and could seriously damage the sterilizer.

The manufacturer's warranty is void in case of damage from chemicals coming from the load or added to it.

Preparing the trays

Do not overload the chamber; adhere to the maximum load weight limits (see cycle program table; the available sterilization cycles).

Always use the chamber rack to allow adequate steam circulation.

Place pouched items on trays with the paper side facing up.

Do not overload trays. The weight must be spread as evenly as possible among the trays.

Place cassettes in the vertical position (if possible) to enhance drying.

Place empty containers or non-perforated trays upside down to prevent accumulation of water.

Items made from different materials (stainless steel, carbon steel, aluminum, etc.) must be placed on separate trays or wrapped/pouched.

If the instruments are manufactured from carbon steel, paper should be placed between them and the trays to avoid rusty spots.


Sterilize hinged instruments (e.g., forceps, extraction pliers, etc.) in the open position.

Wrap items with porous wrapping materials to facilitate steam penetration and drying (e.g. sterilization bags for autoclaves).

Loading the chamber

Tubes

Rinse, drain and dry tubes after washing. Place tubes on a tray allowing the ends to remain open. Do not bend tubes.

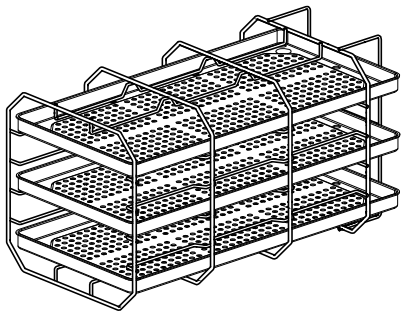

Partial loads


If the chamber is just partially loaded, place the load in such a way that the space in-between the trays is maximized (see example with three trays on the left).

Wrapped/bagged items

Place the bags on trays allowing adequate space in-between bags.


Ensure that packs do not touch the sterilizer chamber walls.

Place sterilization bags with the paper side facing up.

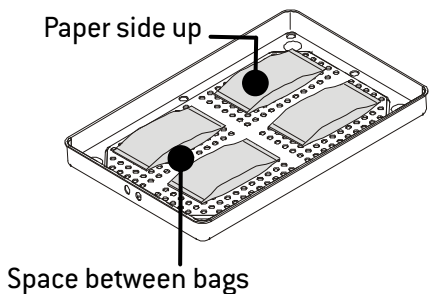

Never place the load or the trays directly into the chamber without the chamber rack as this could affect the steam and temperature distribution. The load must always be supported by the chamber rack.

Before initiating a sterilization cycle, always check that the steam diffuser plate is properly positioned.

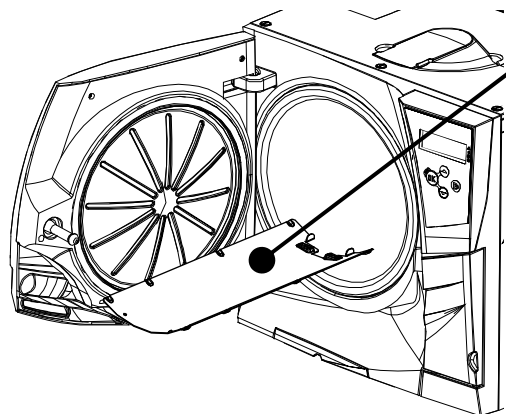

An improper positioning of the steam diffuser plate could result in bad steam quality and could impair the sterilization process, with risk of non sterile load and cross infection. Sterility at the end of the cycle is not guaranteed if the steam diffuser plate was not correctly placed.



Before touching, ensure the sterilization chamber is cold: risk of burns!

ANNEX 4. Bowie and Dick test


Description

The Bowie & Dick (B&D) test device is used to validate the sterilizer performance for textile load sterilization. It is made of several sheets of paper wrapped in a small packet in the middle of which there is a chemical heat-sensitive indicator sheet.


How to carry out the test

The test must be performed in an empty chamber (EN13060) without load but with the standard chamber accessories (chamber rack and trays) mounted.

Place the Bowie & Dick test pack in the center of a tray in the lowest rack position.

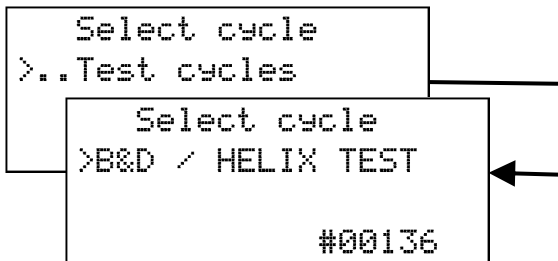


Use the UP, DOWN and OK buttons to browse the menu, choosing the following options in sequence: MENU – TEST CYCLES – B&D/HELIX TEST
Initiate the cycle (see “Running a sterilization cycle”).
Once the cycle is finished, remove the test pack from the chamber.
Remove the indicator sheet from the center of the test pack and check the change in colour:

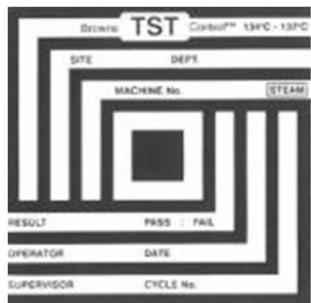

TEST PASSED

The entire surface of the indicator sheet has changed colour.

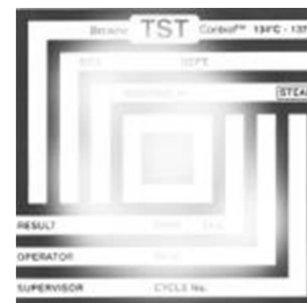

TEST FAILED

Certain areas of the indicator sheet have not changed colour, e.g., the central part has not turned dark due to an air pocket in the center of the test pack.



The test pack will be very hot at the end of the cycle! It is normal that the test pack is wet.


Test failure indicates that there was an air pocket present during the cycle due to sterilizer malfunction.

If the test fails repeatedly call technical service.

Follow local/national guidelines on the frequency of testing.



ANNEX 5. Helix test


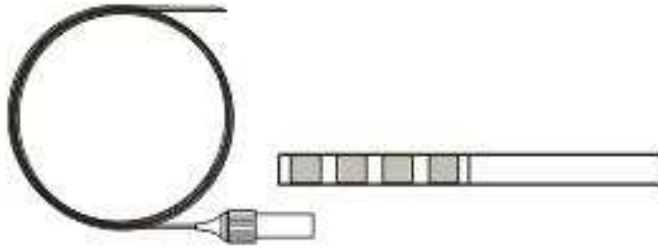


Description

The Helix test device is used to validate the sterilizer performance for hollow items. It consists of a 1,500 mm long tube that is open on one side and closed with a capsule on the other side. A chemical indicator strip is placed inside of the capsule.

How to carry out the test

The test must be performed in an empty chamber (EN13060) without load. Remove all trays except the lowest one. Place an indicator strip inside the capsule according to the instructions of the test manufacturer. Close the capsule. Place the test device in the centre of the lowest tray.

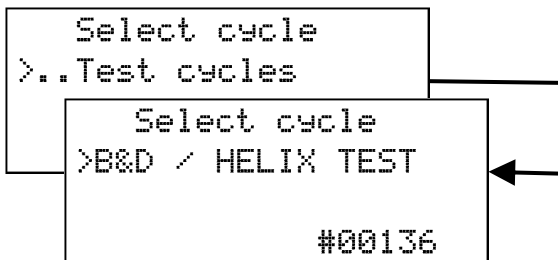

Use the UP, DOWN and OK buttons to browse the menu, choosing the following options in sequence: MENU – TEST CYCLES – B&D/HELIX TEST
Initiate the cycle (see “Running a sterilization cycle”).
Once the cycle is finished, remove the test device from the chamber.
Remove the indicator strip from the capsule and check the change in colour:



The indicator strip has turned dark.



Part of the chemical indicator strip has not turned dark; e.g. due to residual air inside the capsule.



Test failure indicates that there was an air pocket present during the cycle due to sterilizer malfunction.
If the test fails repeatedly call technical service.
Follow local/national guidelines on the frequency of testing.

ANNEX 6. Vacuum test

Description

The vacuum test is designed to validate the sterilizer performance in terms of:


- Efficiency of the vacuum pump;
- Tightness of the pneumatic circuit.

It consists of a vacuum phase, followed by a stabilization period of 5 minutes and a testing period of 10 minutes.

During the 10-minute testing period the internal pressure is monitored. The pressure rise must be less than 0.013 bar.


How to carry out the test

The test must be performed when the **sterilizer chamber is completely dry and cold** as otherwise the test could produce a “false negative” outcome.

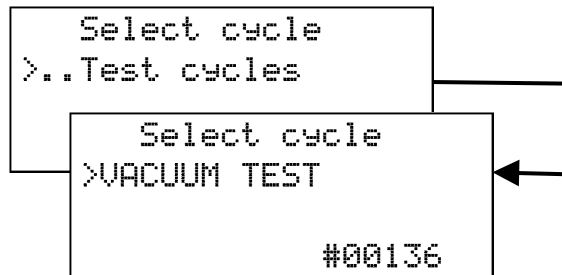

Use the UP, DOWN and OK buttons to browse the menu, choosing the following options in sequence: MENU – TEST CYCLES – VACUUM TEST

Initiate the cycle (see “Running a sterilization cycle”).

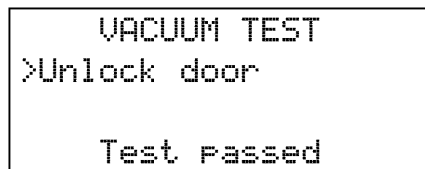

Once the cycle is finished, you will be able to open the chamber door.

A display message will inform if the test passed or failed.



If the test failed, check, clean or replace the door gasket, clean the chamber face side and the chamber filter; repeat the test.

If the test fails repeatedly call technical service.

Follow local/national guidelines on the frequency of testing.

ANNEX 7. Water quality

LINA sterilizers use distilled or demineralized water to generate steam for the sterilization process.

The table below lists the maximum content of minerals and the specifications for the water used for steam sterilization (see EN13060 ANNEX C).

| FEED WATER SPECIFICATIONS | |
|--|--|
| Contaminants/minerals/qualities | Value/Specification |
| Evaporate residue | < 10 mg/l |
| Silicon oxide, SiO ₂ | < 1 mg/l |
| Iron | < 0,2 mg/l |
| Cadmium | < 0,005 mg/l |
| Lead | < 0,05 mg/l |
| Heavy metals (excl. iron, cadmium, lead) | < 0,1 mg/l |
| Chloride | < 2 mg/l |
| Phosphate | < 0,5 mg/l |
| Conductivity (at 20°C) | < 15 µs/cm |
| pH value | 5 - 7 |
| Appearance | colorless, clean, free from sediment |
| Hardness | < 0,02 mmol/l |
| Chemical additives | No chemicals or additives must be added to the water used for the steam sterilization process, even if they are specifically claimed for use in steam generators, or for steam production, or as additives for sterilization, disinfection, cleaning or corrosion protection. |



The use of water with a conductivity greater than 15µS/cm may affect the sterilization process and damage the sterilizer.

The use of water with a conductivity greater than 50µS/cm, or not complying with the specifications in the table above, may strongly affect the sterilization process and seriously damage the sterilizer.

The manufacturer's warranty is void if the sterilizer was used with water containing contaminant or chemical levels exceeding those listed in the table above.

ANNEX 8. Example of cycle data report

| | | | | | |
|---|---|-------------------|-------------|------------|--------------|
| Sterilizer brand | → | W&H Sterilization | | | |
| Sterilizer model and serial number | → | LINA PRO13-003-17 | | | 125415 |
| ----- | | | | | |
| Surgery – practice – doctor name | → | Dr. Smith | | | |
| Cycle name | → | Cycle: | B UNIVERSAL | 134 | |
| Cycle counter | → | Number: | | 1898 | |
| Programmed sterilization temperature | → | Sterilizat. temp | | 134.0°C | |
| Programmed sterilization time | → | Sterilizat. time | | 04:00 | |
| Programmed drying time | → | Drying time | | 15:00 | |
| Cycle start date and time | → | Date/time: | 02/05/2015 | 10:12 | |
| Headers for the table below | → | Phase | Time | part. | T °C P Bar |
| ----- | | | | | |
| Cycle start | → | Start | 00:00 | 00:00 | 20.4 0.00 |
| Pre-heating phase | → | HEA | 08:17 | 08:17 | 90.9 0.02 |
| Pressure and vacuum pulses | → | PV1 | 10:14 | 01:57 | 53.5 -0.86 |
| | | PP1 | 13:00 | 02:46 | 102.7 0.15 |
| | | PV2 | 15:45 | 02:45 | 57.7 -0.83 |
| | | PP2 | 18:58 | 03:13 | 102.7 0.15 |
| | | PV3 | 21:50 | 02:52 | 62.2 -0.83 |
| Phase of pressure rise to sterilization conditions | → | PPH | 30:48 | 08:58 | 134.5 2.11 |
| ----- | | | | | |
| Sterilization phase (process) start | → | PRs | 30:48 | 00:00 | 134.5 2.11 |
| Min. and max. temperatures during the sterilization phase (process) | → | Min. | 00:00 | | 134.5 ---- |
| | | Max. | 02:24 | | 135.4 ---- |
| Min. and max. pressures during the sterilization phase (process) | → | Min. | 00:00 | | ---- 2.11 |
| | | Max. | 02:21 | | ---- 2.16 |
| Process end conditions | → | Pre | 34:48 | 04:00 | 135.3 2.15 |
| ----- | | | | | |
| Drying phase start | → | DRVs | 34:48 | 00:00 | 135.3 2.17 |
| Drying phase end | → | DRVe | 49:48 | 15:00 | 70.9 -0.86 |
| ----- | | | | | |
| Chamber venting phase | → | VEN | 50:48 | 01:00 | 73.8 -0.01 |
| Pressure leveling phase | → | LEU | 50:49 | 00:01 | 73.9 -0.01 |
| Cycle end conditions | → | END | 50:49 | 00:00 | 73.9 -0.01 |
| ----- | | | | | |
| Cycle end date and time | → | Date/time: | | 02/05/2015 | 11:03 |
| Cycle outcome | → | | | Cycle | completed |
| ----- | | | | | |
| Tracking code for traceability management | → | Trk: | | | CC18A8800084 |




NOTE

Use only the printer and the thermal paper provided by W&H. This ensures a long (at least 10 years) stability of image of the printouts.


ANNEX 9. Accessories and spare parts




Printer model S'Print
part n. 19721108




Label printer LisaSafe
part n. 19721100 (label printer only)
part n. 19721102 (LisaSafe Connection Kit)




USB + serial kit
part n. X051124x




USB pen drive
part n. V000004x




Automatic water feed and drain kit
part n. X051110x



Permanent drain kit
part n. X051052x



Drain tube kit with fittings
part n. A812110x




Dust filter
part n. F364502x



QR code reader / bar code reader
part n. 19721132



Aluminium tray
LINA17: part n. F523204x
LINA 22: part n. F523205x



Tray holder
part n. F523001x




Funnel
part n. F540903x



Bacteriological filter
part n. W322400x




Door seal
part n. F460504x




Wall spacer
part n. F190107x



Safety bracket kit
part n. X051019x




Drain tube
part n. S230900x



Mains cable
part n. U38010xx

Accessories

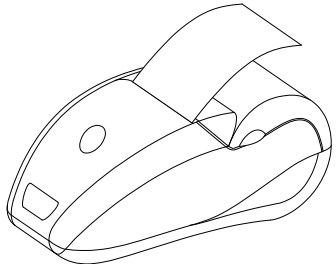

Cycle report printer (S'Print) - part n. 19721108

S'Print is a compact, reliable and easy-to-use printer that can be connected directly to the serial port located in the rear of the sterilizer.

S'Print can be easily managed from the sterilizer control panel (See Chapter 5 - Programming) in order to:

- Print cycle data reports (see ANNEX 8 “Example of a cycle data report”) at the end of each cycle either in automatic or manual print mode;
- Print a report of any cycle stored in the sterilizer memory.


Printouts are very durable (more than 10 years).

LisaSafe traceability system

Label printer - part n. 19721100

Connection kit and consumables - part n. 19721102

QR code / bar code reader reader - part n. 19721132

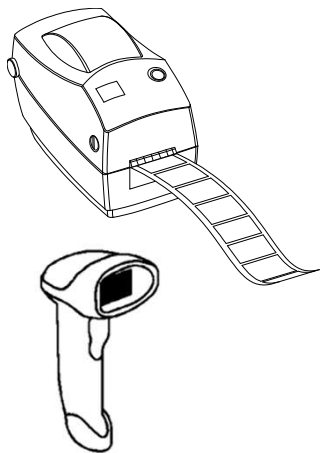

LisaSafe is a fast label printer that can be connected directly to the serial port located in rear of the sterilizer.

LisaSafe prints self-adhesive permanent paper labels to be attached to pouches, showing:

- either the main information of the cycle and the sterile load (cycle number and type, date, time, expiry date);
- or the sterilization lot number.


LisaSafe is conceived to be the heart of the traceability system in the dental practice, permitting a safe and easy management of the stock of sterilized tools and instruments.

LisaSafe is also compatible with the W&H sterilizers series 300, 500 and 500 Fully Automatic.

All the label printer functions can be easily controlled from the sterilizer control panel (See Chapter 5 - Programming) in order to:

- Print a selected number of labels at the end of the cycle, either in automatic or manual print mode;
- Print extra labels of the most recent cycle;
- Print labels of any cycle stored in the sterilizer memory.


Accessories

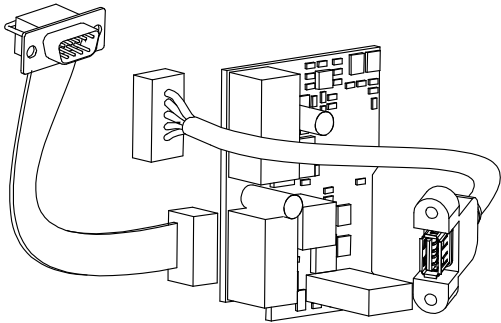

USB port + additional serial port kit - part n. X051124x

Mount this kit if you want to connect a USB pen drive to save the cycle reports, or an additional serial device (e.g. a label printer).

The kit must be installed by an authorized service technician, or by the factory upon specific order request.

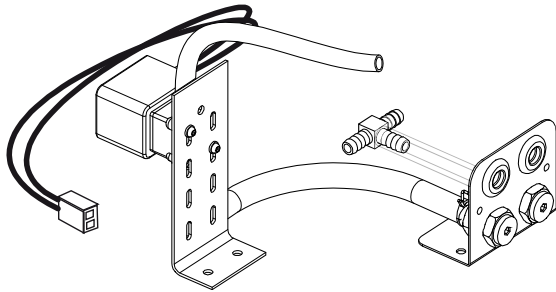


Water feed system - part n. X051110x

Mount this kit in the sterilizer if you want to connect a water filtration system to automatically fill the clean water tank with demineralized water and drain the used water tank continuously.

The kit needs to be mounted by an authorized service technician, or by the factory upon specific order request.


Water quality provided by the filtration system has to comply with ANNEX 7. The water supply pressure must be between 2 and 8,6 bar.

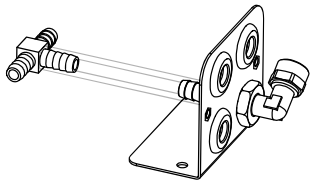

Permanent drain kit - part n. X051052x

This kit is mounted to continuously drain the used water tank, thus manual tank draining is no longer necessary.

The kit needs to be mounted by an authorized service technician, or by the factory upon specific order request.

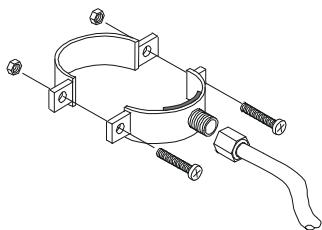


Drain tube kit with fittings - part n. A812110x


Use this kit to connect the sterilizer permanent drain to a drain pipe.

Accessory connection schemes


Data communication

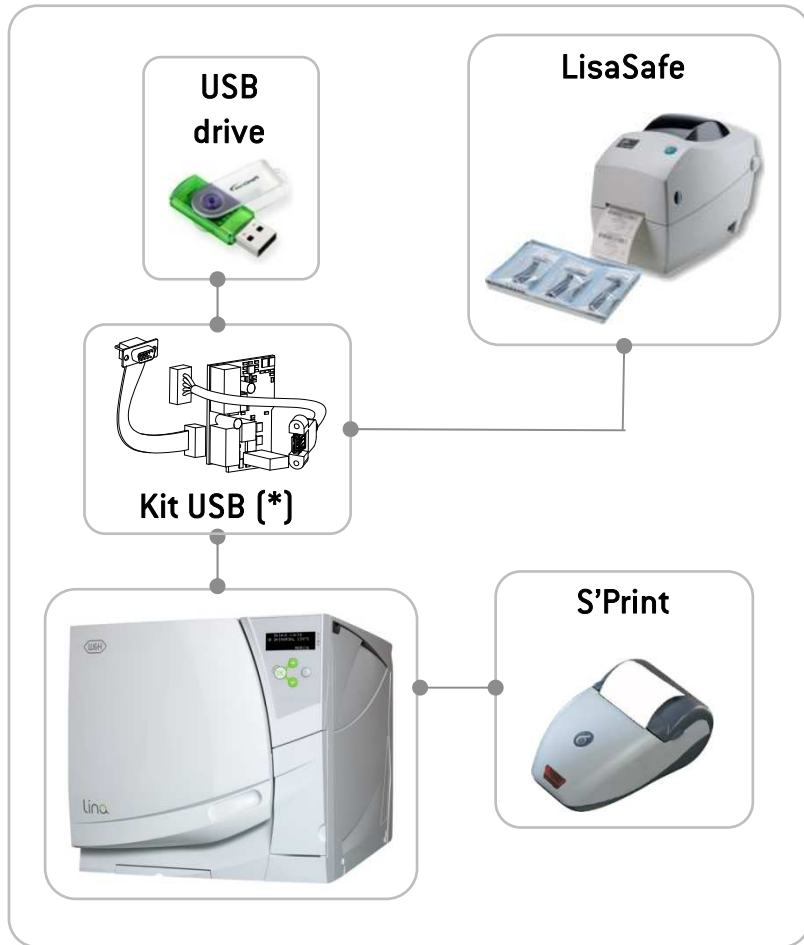

(*) Rear serial connections (with USB kit)


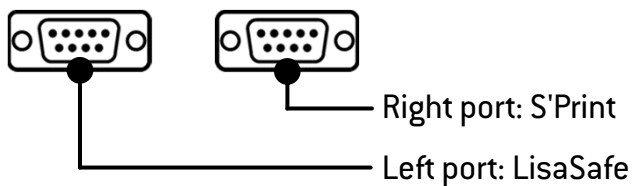


Water treatment, supply and drain


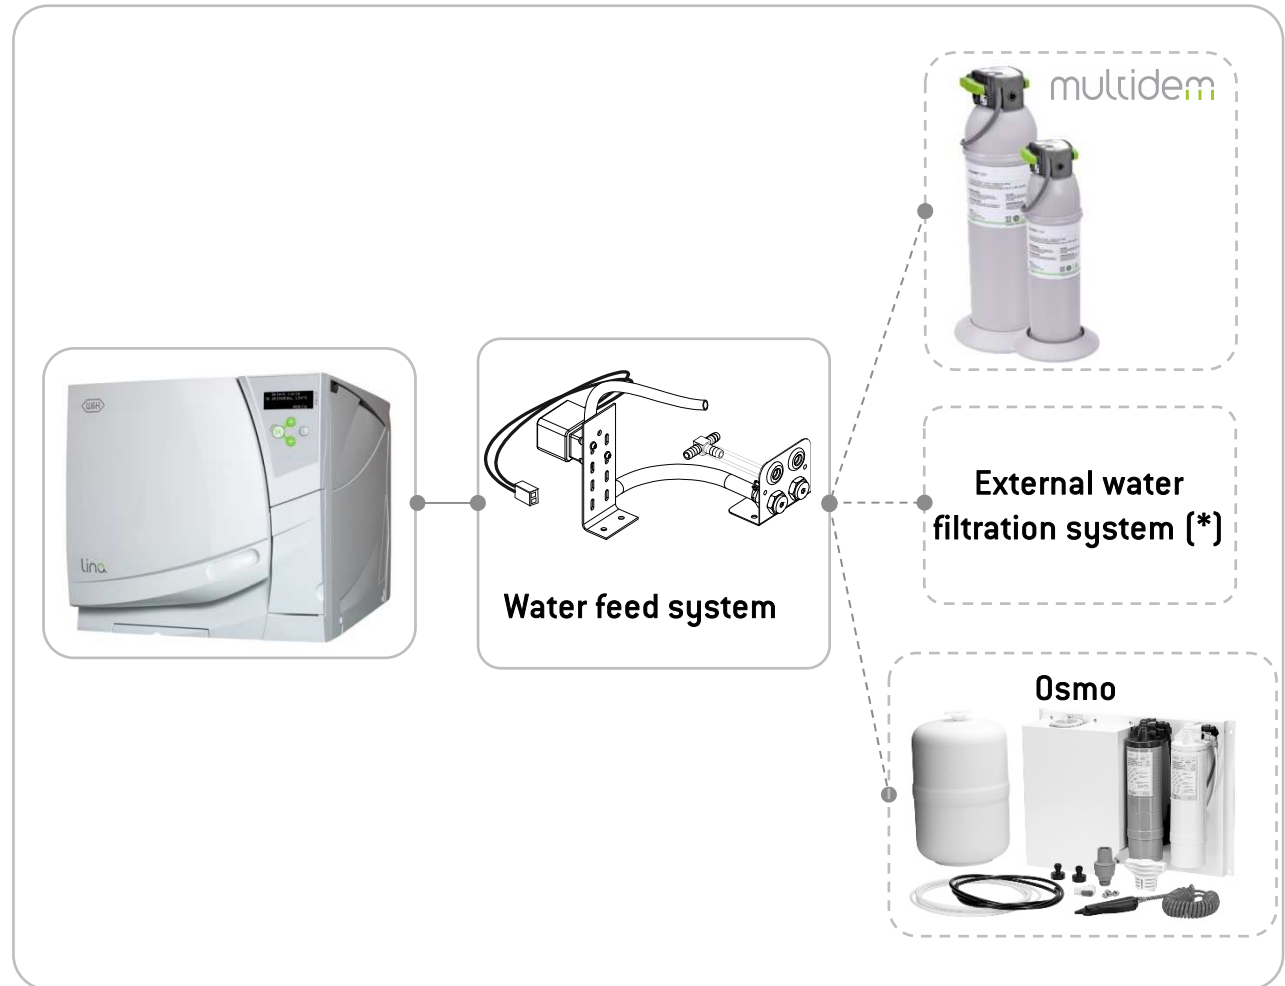


(*) The water filtration system must be fitted with a backflow preventing device complying to IEC 61770 and to national and local regulations.
Maximum pressure 8.6 bar, minimum flow 2.5 litres/min., max. temperature 35 °C.



Accessories and spare parts





Standard chamber rack for 3 cassettes (*)
LINA 17: part n. F523008x
LINA 22: part n. F523009x



Standard chamber rack for 3 USA size cassettes (*)
LINA 17: part n. F523020x
LINA 22: part n. F523021x




Standard chamber rack for 4 cassettes (*)
LINA 17: part n. F523012x
LINA 22: part n. F523015x




Standard chamber rack for 2 implant cassettes (*)
LINA 17: part n. F523016x
LINA 22: part n. F523017x

(*) All racks shown in this page, if rotated 90°, accept 5 standard aluminium trays.


Consumables




Bacteriological filter - part n. W322400x
Replace every 400 cycles



Door seal - part n. F460504x
Replace every 800 cycles



Dust filter - part n. F364502x
Replace every 400 cycles

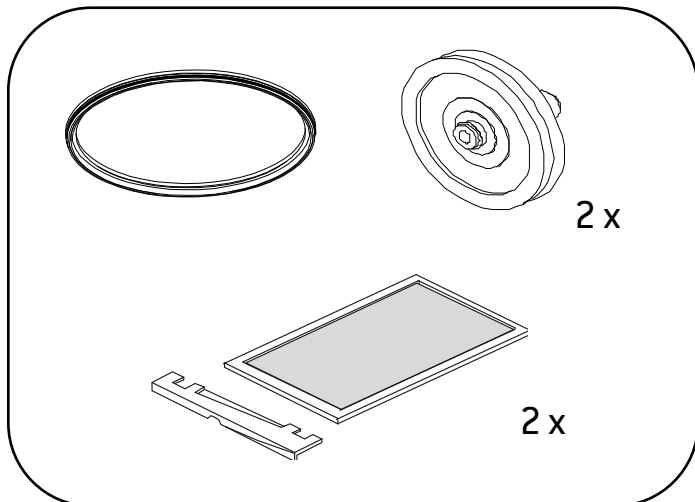

400-800 cycle consumable kit - part n. X050315x

This kit consists in a stock of consumables suitable to run 800 cycles.

It includes:

- 1 door seal;
- 2 air filters;
- 2 dust filters with handle.

ANNEX 10. Helix test documentation form

Use this page to create a logbook tracing the effectiveness of the sterilization cycle during the whole lifespan of your sterilizer.

| Date | Cycle N. | Operator | Released | | Signature | Chemical indicator |
|------|----------|----------|----------|----|-----------|--------------------|
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |
| | | | YES | NO | | |

APPENDIX 11. W&H Installation check-list

| | | | |
|----|--|-----|----|
| 1 | Was the head of the clinic/practice present during all the in-service? | Yes | No |
| 2. | Is the packing of the sterilizer undamaged? | Yes | No |
| 3 | When unpacked, is the sterilizer undamaged? | Yes | No |
| 4 | Are all the contents of the package available (sterilizer ship-with)? | Yes | No |
| 5 | Are all the ordered accessories available with the sterilizer? | Yes | No |
| 6 | Have you removed all the protection covers from the sterilizer and from all the ship-with? | Yes | No |
| 7 | Were all sections of the instruction for use of the sterilizer covered and explained during the in-service? | Yes | No |
| 8 | Is the allocated countertop for the sterilizer, levelled and flat? | Yes | No |
| 9 | Are the recommended ventilation indications of the allocated area for the sterilizer, respected? | Yes | No |
| 10 | Are the required minimum clearances respected? | Yes | No |
| 11 | Have you explained, which water quality required for the use of the sterilizer is? Check and measure the μS of the water. | Yes | No |
| 12 | Have you shown to the head of the clinic/practice the procedure for filling and draining the main and used water tanks? | Yes | No |
| 13 | Have you shown to the head of the clinic/practice how to program the sterilizer? | Yes | No |
| 14 | Have you shown to the head of the clinic/practice the cycle options? | Yes | No |
| 15 | Have you shown to the head of the clinic/practice what the Messages and Alarms mean? | Yes | No |
| 16 | Have you shown to the head of the clinic/practice how to manually abort a cycle? | Yes | No |
| 17 | Have you shown to the head of the clinic/practice the maintenance program and procedures? | Yes | No |
| 18 | Have you shown to the head of the clinic/practice how to use all of the accessories? | Yes | No |
| 19 | Have you shown to the head of the clinic/practice the advantages of having a USB connection for a pen drive? | Yes | No |
| 20 | Have you suggested to the head of the clinic/practice to periodically backup the data, stored on the USB pen drive, on another safe support? | Yes | No |

W&H Installation check-list

- | | | | |
|----|---|-----|----|
| 21 | Have you executed a Vacuum test? | Yes | No |
| 22 | Have you executed a B Universal 134°C cycle program with the tray rack and trays inserted? | Yes | No |
| 23 | Have you explained to the head of the clinic/practice the correct load type for each available sterilization program? | Yes | No |
| 24 | Have you shown to the head of the clinic/practice how to prepare and place the load in the sterilizer chamber? | Yes | No |
| 25 | Have you explained to the head of the clinic/practice to use only original parts and accessories on the sterilizer? | Yes | No |
| 26 | Have you shown and explained to the head of the clinic/practice the safety advise section? | Yes | No |
| 27 | Are all connections to the sterilizer well positioned and plugged (accessories, etc...)? | Yes | No |

Sterilizer Serial Number: _____

Date: _____ Purchased From: _____ Installed By: _____

Dr./Clinic Name: _____ Address: _____ Phone: _____

Receiver's Signature: _____ Installer's Signature: _____

Upon completion of the Installation Checklist please fax a copy to W&H

Fax: +43 6274 6236-55 OR

Make a copy of the Installation Checklist and mail it to:

Ignaz-Glaser-Straße 53, Postfach 1

5111 Bürmoos - Austria

Authorized W&H service partners

A list and a map with your nearest W&H service partner are available at <http://wh.com>

Manufacturer

W&H Sterilization S.r.l.
Italy, I-24060 Brusaporto (Bg), via Bolgara, 2

t +39/035/66 63 000 f +39/035/50 96 988
wh.com

LINA PR013-003 ENG - Rev. 7



Subject to alterations

15.02.2022